

**METTLER TOLEDO**



# Table of Contents

<b>1</b>	<b>Introduction</b>	<b>7</b>
1.1	Document purpose .....	7
1.2	Further documents and information .....	7
1.3	Explanation of conventions and symbols used .....	7
1.4	Acronyms and abbreviations .....	8
1.5	Product range .....	8
1.5.1	MR analytical balances .....	8
1.5.2	MR precision balances .....	9
<b>2</b>	<b>Safety Information</b>	<b>10</b>
2.1	Definition of signal words and warning symbols .....	10
2.2	Product-specific safety notes .....	10
<b>3</b>	<b>Design and Function</b>	<b>12</b>
3.1	Overview analytical balances .....	12
3.2	Overview precision balances, with draft shield .....	13
3.3	Overview precision balances, without draft shield .....	13
3.4	Overview terminal .....	14
3.5	Overview interface connections .....	14
3.6	Components description .....	15
3.6.1	Draft shield .....	15
3.6.2	Weighing pan .....	15
3.6.3	Drip tray .....	15
3.6.4	Door handle .....	15
3.6.5	Leveling feet .....	16
3.6.6	Terminal .....	16
3.6.7	QuickLock for draft shield .....	16
3.6.8	QuickLock for doors and front panel .....	16
3.6.9	Release button for back panel .....	17
3.7	Overview type label .....	17
3.8	User interface .....	18
3.8.1	Main sections at a glance .....	18
3.8.2	Main weighing screen .....	18
3.8.3	Balance menu .....	19
3.8.4	Main configuration .....	20
3.8.5	Applications .....	20
3.8.6	Icons and symbols .....	21
3.8.6.1	System status icons .....	21
3.8.6.2	Weighing status icons .....	21
3.8.6.3	Process status icons .....	21
<b>4</b>	<b>Installation and Putting into Operation</b>	<b>23</b>
4.1	Selecting the location .....	23
4.2	Unpacking the balance .....	23
4.3	Installation .....	24
4.3.1	Balances with draft shield .....	24
4.3.2	Balances without draft shield .....	27
4.4	Putting into operation .....	27
4.4.1	Connecting the balance .....	27
4.4.2	Switching on the balance .....	28
4.4.3	Leveling the balance .....	28
4.4.4	Performing an internal adjustment .....	28
4.4.5	Entering / Exiting standby mode .....	29
4.4.6	Entering / Exiting power-saving mode .....	29
4.4.7	Switching off the balance .....	29

4.5	Performing a simple weighing .....	29
4.5.1	Opening and closing draft shield doors .....	29
4.5.2	Zeroing the balance.....	30
4.5.3	Taring the balance .....	30
4.5.4	Performing a weighing .....	30
4.6	Transporting, packing, and storing .....	30
4.6.1	Transporting the balance over short distances .....	30
4.6.2	Transporting the balance over long distances .....	31
4.6.3	Packing and storing .....	31
4.7	Weighing below the balance.....	31
<b>5</b>	<b>Operation</b> .....	<b>32</b>
5.1	Touchscreen .....	32
5.1.1	Selecting or activating an item .....	32
5.1.2	Scrolling .....	32
5.1.3	Opening the fly-in panel.....	32
5.1.4	Entering characters and numbers.....	32
5.1.5	Changing values.....	33
5.1.6	Sliding .....	34
5.2	General balance settings .....	34
5.2.1	Date / Time / Language .....	34
5.2.2	Screen / Sound .....	34
5.2.3	Standby, Power-saving mode.....	34
5.2.4	Weighing / Quality .....	35
5.2.4.1	Warnings and reminders .....	35
5.2.4.2	Weighing profiles.....	35
5.2.4.2.1	Environment.....	36
5.2.4.2.2	Weighing mode.....	36
5.2.4.2.3	Value release .....	36
5.3	Weighing applications .....	36
5.3.1	Weighing applications overview .....	36
5.3.2	General settings for weighing applications .....	37
5.3.2.1	Defining target weight and tolerances .....	37
5.3.2.2	Defining a sample ID.....	37
5.3.2.3	Configuring a weighing application .....	38
5.3.2.4	Configuring a weighing series .....	38
5.3.2.5	Using automated functions.....	39
5.3.2.6	Configuring a report .....	39
5.3.3	Application "Weighing" .....	40
5.3.4	Application "Counting" .....	40
5.3.5	Application "Check weighing" .....	41
5.3.6	Application "Dynamic weighing" .....	42
5.3.7	Application "Formulation" .....	43
5.3.8	Application "Totaling" .....	44
5.3.9	Application "Back weighing" .....	44
5.3.10	Application "Density" .....	45
5.4	Adjustments.....	46
5.4.1	Adjustment strategy .....	46
5.4.2	Editing an adjustment.....	46
5.4.3	Performing an internal adjustment .....	47
5.4.4	Performing an external adjustment .....	47
5.5	Tests.....	47
5.5.1	Editing a test .....	47
5.5.2	Performing a test .....	48
5.5.2.1	Sensitivity test.....	48
5.5.2.2	Repeatability test.....	48
5.5.2.3	Eccentricity test.....	49
5.6	Interfaces .....	50

5.6.1	Ethernet .....	50
5.6.2	Bluetooth .....	50
5.7	Devices / Printers .....	50
5.7.1	Printer .....	51
5.7.1.1	Installing a printer through RS232 .....	51
5.7.1.2	Installing a printer through Bluetooth .....	52
5.7.2	Barcode reader .....	53
5.7.2.1	Scanning a sample ID with a barcode reader .....	53
5.7.3	Foot switch .....	53
5.7.4	Keyboard .....	54
5.7.5	Adding and deleting a device .....	54
5.7.6	Editing the settings of a device .....	55
5.8	Services .....	55
5.8.1	MT-SICS service .....	55
5.8.2	EasyDirect Balance .....	56
5.8.3	Drop to cursor .....	56
5.9	Publishing .....	57
5.9.1	Printing data .....	57
5.9.1.1	Printing results manually through USB .....	57
5.9.1.2	Printing results automatically through Bluetooth .....	58
5.9.2	Exporting data to a USB storage device .....	58
5.9.3	Transferring data to services .....	58
5.9.3.1	Transferring data: Drop to cursor .....	59
5.9.3.2	Transferring data: MT-SICS service .....	59
5.9.3.3	Transferring data: EasyDirect Balance .....	60
5.9.4	Publishing options .....	61
5.10	User management .....	61
5.10.1	Activating / deactivating the user management .....	61
5.10.2	Managing users and user groups .....	61
5.10.2.1	Automatic logout .....	61
5.10.2.2	Creating a new user .....	62
5.10.2.3	Deleting a user .....	62
5.10.2.4	Managing groups .....	62
5.11	Password protection .....	63
5.11.1	Logging in and logging out .....	63
5.11.2	Changing a password .....	63
5.11.3	Resetting a password .....	63
5.12	Approved balances .....	64
5.12.1	Definitions .....	64
5.12.2	Descriptive markings .....	64
5.12.3	Restrictions on zeroing and taring .....	64
5.12.4	Application: Weighing .....	64
5.12.5	Representation of weighing results .....	65
5.12.6	MT-SICS .....	65
5.12.7	Reference .....	65
<b>6</b>	<b>Software Description</b> .....	<b>66</b>
6.1	Balance menu settings .....	66
6.1.1	Leveling aid .....	66
6.1.2	History .....	66
6.1.2.1	Adjustments history .....	66
6.1.2.2	Tests history .....	67
6.1.2.3	Service history .....	67
6.1.2.4	Activity log .....	67
6.1.2.5	Software update history .....	67
6.1.2.6	Error log .....	68
6.1.3	Information .....	68
6.1.3.1	Balance information .....	68

6.1.3.2	Service and support information .....	68
6.1.4	User management.....	68
6.1.4.1	User management – General .....	69
6.1.4.2	User management – Users .....	69
6.1.4.3	User management – Groups.....	69
6.1.5	Settings .....	70
6.1.5.1	Settings: Balance .....	70
6.1.5.1.1	Settings: Weighing / Quality .....	70
6.1.5.1.2	Settings: Publishing .....	72
6.1.5.1.3	Settings: Date / Time / Language .....	73
6.1.5.1.4	Settings: Screen / Sound .....	73
6.1.5.1.5	Settings: General .....	74
6.1.5.2	Settings: Interfaces .....	74
6.1.5.2.1	Settings: Ethernet .....	74
6.1.5.2.2	Settings: Bluetooth .....	75
6.1.5.3	Settings: Devices / Printers.....	75
6.1.5.4	Settings: Services.....	75
6.1.5.4.1	Settings: MT-SICS service.....	75
6.1.5.4.2	Settings: EasyDirect Balance .....	76
6.1.5.4.3	Settings: Drop to cursor .....	76
6.1.6	Maintenance .....	76
6.2	Weighing applications settings .....	77
6.2.1	Settings: application "Weighing" .....	77
6.2.1.1	Main configuration .....	77
6.2.1.2	ID format .....	78
6.2.1.3	Weighing configuration.....	78
6.2.1.4	Automation .....	79
6.2.1.5	Report configuration .....	79
6.2.2	Settings: application "Counting" .....	79
6.2.2.1	Main configuration .....	80
6.2.2.2	ID format .....	80
6.2.2.3	Weighing configuration.....	80
6.2.2.4	Automation .....	81
6.2.2.5	Report configuration .....	81
6.2.3	Settings: application "Check weighing" .....	82
6.2.3.1	Main configuration .....	82
6.2.3.2	ID format .....	82
6.2.3.3	Weighing configuration.....	83
6.2.3.4	Automation .....	83
6.2.3.5	Report configuration .....	84
6.2.4	Settings: application "Dynamic weighing" .....	84
6.2.4.1	Main configuration .....	84
6.2.4.2	ID format .....	85
6.2.4.3	Weighing configuration.....	85
6.2.4.4	Automation .....	85
6.2.4.5	Report configuration .....	86
6.2.5	Settings: application "Formulation" .....	86
6.2.5.1	Main configuration .....	86
6.2.5.2	ID format .....	87
6.2.5.3	Weighing configuration.....	87
6.2.5.4	Automation .....	87
6.2.5.5	Report configuration .....	87
6.2.6	Settings: application "Totaling" .....	88
6.2.6.1	Main configuration .....	88
6.2.6.2	ID format .....	88
6.2.6.3	Weighing configuration.....	89
6.2.6.4	Automation .....	89

6.2.6.5	Report configuration .....	89
6.2.7	Settings: application "Back weighing" .....	89
6.2.7.1	Main configuration .....	90
6.2.7.2	ID format .....	90
6.2.7.3	Weighing configuration .....	91
6.2.7.4	Automation .....	91
6.2.7.5	Report configuration .....	92
6.2.8	Settings: application "Density" .....	92
6.2.8.1	Main configuration .....	92
6.2.8.2	ID format .....	93
6.2.8.3	Weighing configuration .....	93
6.2.8.4	Report configuration .....	94
6.3	Adjustment settings .....	94
6.3.1	Settings: Adjustment strategy .....	94
6.3.2	Settings: Internal adjustment .....	94
6.3.3	Settings: External adjustment .....	95
6.4	Test settings .....	95
6.4.1	Settings: Sensitivity test .....	96
6.4.2	Settings: Repeatability test .....	96
6.4.3	Settings: Eccentricity test .....	97
<b>7</b>	<b>Maintenance</b> .....	<b>99</b>
7.1	Maintenance tasks .....	99
7.2	Cleaning .....	99
7.2.1	Disassembling for cleaning .....	99
7.2.1.1	Balances with draft shield .....	99
7.2.1.2	Balances without draft shield .....	102
7.2.2	Cleaning agents .....	102
7.2.3	Cleaning the balance .....	103
7.2.4	Putting into operation after cleaning .....	104
7.3	Service .....	104
7.4	Software update .....	104
7.4.1	Updating the software .....	104
7.4.2	Putting into operation after software update .....	104
7.5	Resetting the balance .....	105
<b>8</b>	<b>Troubleshooting</b> .....	<b>106</b>
8.1	Error messages .....	106
8.2	Error symptoms .....	107
8.3	Saving a support file .....	110
8.4	Putting into operation after fixing an error .....	110
<b>9</b>	<b>Technical Data</b> .....	<b>111</b>
9.1	General data .....	111
9.2	Model-specific data .....	112
9.2.1	Analytical balances, readability 0.1 mg .....	112
9.2.2	Precision balances, readability 1 mg .....	113
9.2.3	Precision balances, readability 10 mg or 100 mg .....	114
9.3	Dimensions .....	116
9.3.1	MR analytical balances, readability 0.1 mg .....	116
9.3.2	MR precision balances, readability 1 mg .....	117
9.3.3	MR precision balances, readability 10 mg / 100 mg .....	118
<b>10</b>	<b>Accessories and Spare Parts</b> .....	<b>119</b>
10.1	Accessories .....	119
10.2	Spare parts .....	124
10.2.1	MR analytical balances, readability 0.1 mg .....	124
10.2.2	MR precision balances, readability 1 mg .....	126

10.2.3	MR precision balances, readability 10 mg / 100 mg .....	127
10.2.4	AC/DC adapter, universal .....	128
10.2.5	Packaging .....	129
10.2.5.1	Balances with draft shield .....	129
10.2.5.2	Balances without draft shield.....	130
<b>11</b>	<b>Disposal</b>	<b>131</b>
<b>12</b>	<b>Compliance Information</b>	<b>132</b>
	<b>Index</b>	<b>133</b>

# 1 Introduction

Thank you for choosing a METTLER TOLEDO balance. The balance combines high performance with ease of use.

This document is based on the software version V 1.1.

## EULA

The software in this product is licensed under the METTLER TOLEDO End User License Agreement (EULA) for Software.

When using this product you agree to the terms of the EULA.

▶ [www.mt.com/EULA](http://www.mt.com/EULA)

## 1.1 Document purpose

This Reference Manual provides detailed instructions on how to use the instrument.

## 1.2 Further documents and information

This document is available in other languages online.



▶ [www.mt.com/MR-RM](http://www.mt.com/MR-RM)

Product page:

▶ [www.mt.com/MR-balances](http://www.mt.com/MR-balances)

Instructions for cleaning a balance, "8 Steps to a Clean Balance":

▶ [www.mt.com/lab-cleaning-guide](http://www.mt.com/lab-cleaning-guide)

Search for software:

▶ [www.mt.com/labweighing-software-download](http://www.mt.com/labweighing-software-download)

Search for documents:

▶ [www.mt.com/library](http://www.mt.com/library)

For further questions, please contact your authorized METTLER TOLEDO dealer or service representative.

▶ [www.mt.com/contact](http://www.mt.com/contact)

## 1.3 Explanation of conventions and symbols used

### Conventions and symbols

Key and/or button designations and display texts are shown in graphic or bold text, e.g.,  **Publish**.

 **Note** For useful information about the product.



Refers to an external document.

### Elements of instructions

In this manual, step-by-step instructions are presented as follows. The action steps are numbered and can contain prerequisites, intermediate results and results, as shown in the example. Sequences with less than two steps are not numbered.

- Prerequisites that must be fulfilled before the individual steps can be executed.

1 Step 1

➔ Intermediate result

2 Step 2

➔ Result

## 1.4 Acronyms and abbreviations

Original term	Explanation
AC	Alternating Current
ASTM	American Society for Testing and Materials
DC	Direct Current
EMC	Electromagnetic Compatibility
FCC	Federal Communications Commission
GWP	Good Weighing Practice
ID	Identification
IP	Ingress Protection
LAN	Local Area Network
LPS	Limited Power Source
MAC	Media Access Control
MT-SICS	METTLER TOLEDO Standard Interface Command Set
NA	Not Applicable
OIML	Organisation Internationale de Métrologie Légale (International Organization of Legal Metrology)
RM	Reference Manual
SOP	Standard Operating Procedure
UM	User Manual
USB	Universal Serial Bus
USP	United States Pharmacopeia

## 1.5 Product range

### 1.5.1 MR analytical balances

Balance	Models designation
	Readability: <b>0.1 mg</b> <ul style="list-style-type: none"><li>• MR104</li><li>• MR204</li><li>• MR304</li></ul>

## 1.5.2 MR precision balances

Balance	Models designation
 A white analytical balance with a glass draft shield and a digital display showing 0.000. The brand name 'METTLER TOLEDO' is visible on the front.	Readability: <b>1 mg</b> <ul style="list-style-type: none"><li>• MR203</li><li>• MR303</li><li>• MR503</li><li>• MR603</li></ul>
 A white precision balance with a flat weighing pan and a digital display showing 0.00. The brand name 'METTLER TOLEDO' is visible on the front.	Readability: <b>10 mg / 100 mg</b> <ul style="list-style-type: none"><li>• MR1002</li><li>• MR2002</li><li>• MR3002</li><li>• MR4002</li><li>• MR6002</li><li>• MR6001</li></ul>

## 2 Safety Information

Two documents named "User Manual" and "Reference Manual" are available for this instrument.

- The User Manual is available online in various languages.
- A printed version of the User Manual is delivered with the instrument.
- The Reference Manual is available online. This manual contains a full description of the instrument and its use.
- Keep both documents for future reference.
- Include both documents if you transfer the instrument to other parties.

Only use the instrument according to the User Manual and the Reference Manual. If you do not use the instrument according to these documents or if the instrument is modified, the safety of the instrument may be impaired and Mettler-Toledo GmbH assumes no liability.

### 2.1 Definition of signal words and warning symbols

Safety notes contain important information on safety issues. Ignoring the safety notes may lead to personal injury, damage to the instrument, malfunctions and false results. Safety notes are marked with the following signal words and warning symbols:

#### Signal words

<b>DANGER</b>	A hazardous situation with high risk, resulting in death or severe injury if not avoided.
<b>WARNING</b>	A hazardous situation with medium risk, possibly resulting in death or severe injury if not avoided.
<b>CAUTION</b>	A hazardous situation with low risk, resulting in minor or moderate injury if not avoided.
<b>NOTICE</b>	A hazardous situation with low risk, resulting in damage to the instrument, other material damage, malfunctions and erroneous results, or loss of data.

#### Warning symbols



General hazard



Notice

### 2.2 Product-specific safety notes

#### Intended use

This instrument is designed to be used by trained staff. The instrument is intended for weighing purposes.

Any other type of use and operation beyond the limits of use stated by Mettler-Toledo GmbH without consent from Mettler-Toledo GmbH is considered as not intended.

#### Responsibilities of the instrument owner

The instrument owner is the person holding the legal title to the instrument and who uses the instrument or authorizes any person to use it, or the person who is deemed by law to be the operator of the instrument. The instrument owner is responsible for the safety of all users of the instrument and third parties.

Mettler-Toledo GmbH assumes that the instrument owner trains users to safely use the instrument in their workplace and deal with potential hazards. Mettler-Toledo GmbH assumes that the instrument owner provides the necessary protective gear.

## Safety notes



### **WARNING**

#### **Death or serious injury due to electric shock**

Contact with parts that carry a live current can lead to death or injury.

- 1 Only use the METTLER TOLEDO power cable and AC/DC adapter designed for your instrument.
- 2 Connect the power cable to a grounded power outlet.
- 3 Keep all electrical cables and connections away from liquids and moisture.
- 4 Check the cables and the power plug for damage and replace them if damaged.



### **NOTICE**


#### **Damage to the instrument or malfunction due to the use of unsuitable parts**

- Only use parts from METTLER TOLEDO that are intended to be used with your instrument.

### 3 Design and Function

#### 3.1 Overview analytical balances


0.1 mg

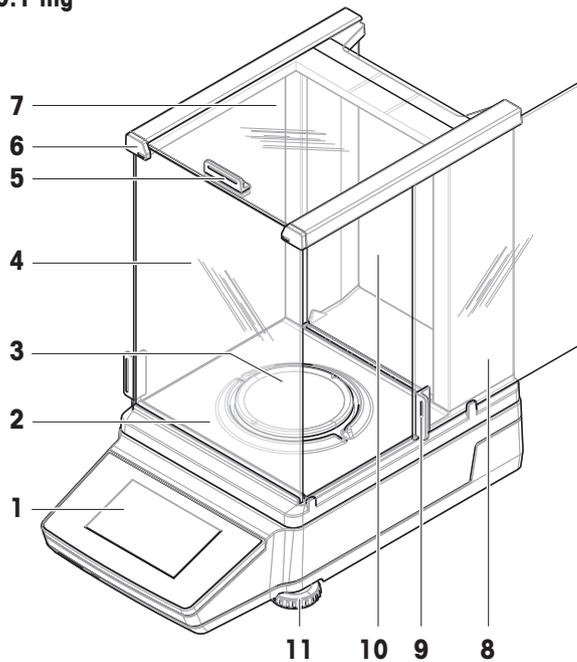

<b>1</b>	Terminal	<b>7</b>	Top door, draft shield
<b>2</b>	Drip tray	<b>8</b>	Side door, draft shield (right/left)
<b>3</b>	Weighing pan	<b>9</b>	Handle, side door
<b>4</b>	Front panel, draft shield	<b>10</b>	Back panel, draft shield
<b>5</b>	Handle, top door	<b>11</b>	Leveling feet
<b>6</b>	QuickLock, doors/panel		

### 3.2 Overview precision balances, with draft shield


1 mg

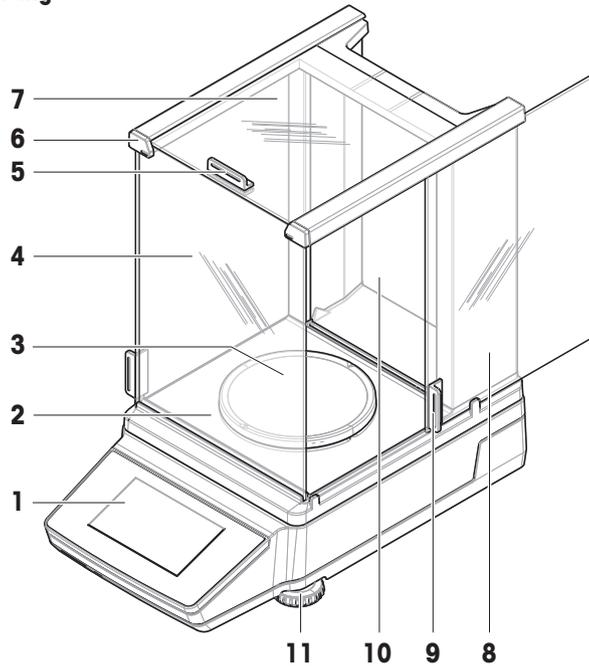

<b>1</b>	Terminal	<b>7</b>	Top door, draft shield
<b>2</b>	Drip tray	<b>8</b>	Side door, draft shield (right/left)
<b>3</b>	Weighing pan	<b>9</b>	Handle, side door
<b>4</b>	Front panel, draft shield	<b>10</b>	Back panel, draft shield
<b>5</b>	Handle, top door	<b>11</b>	Leveling feet
<b>6</b>	QuickLock, doors/panel		


### 3.3 Overview precision balances, without draft shield

10 mg

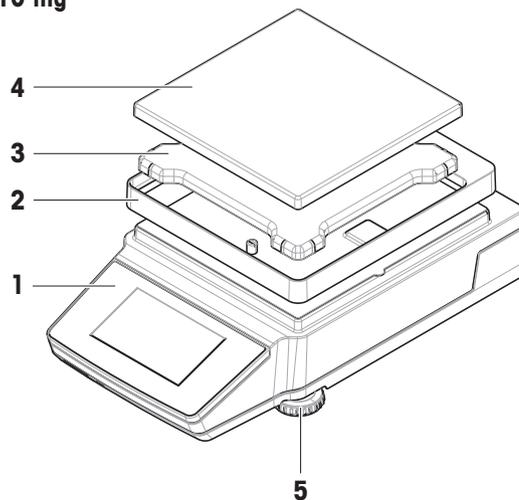


<b>1</b>	Terminal	<b>4</b>	Weighing pan
<b>2</b>	Draft-protection element	<b>5</b>	Leveling feet
<b>3</b>	Weighing pan support		

### 3.4 Overview terminal

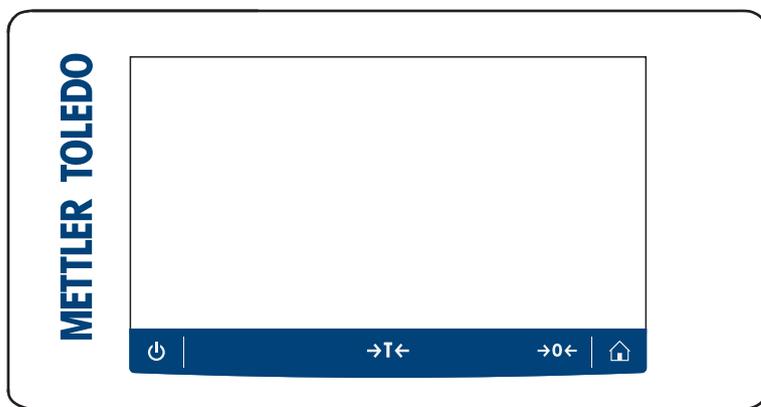

	Name	Description
	<b>Standby / Power-saving mode</b>	By tapping , the balance is not completely switched off but goes into standby mode or power-saving mode. To switch the balance completely off, it must be unplugged from the power supply.  <b>Note</b> Do not disconnect the balance from the power supply unless the balance is not used for an extended period of time. After switching on the instrument, it must warm up before giving accurate results.
	Tare	Tares the balance.  This function is used when the weighing process involves containers. After taring the balance, the screen shows <i>Net</i> which indicates that all displayed weights are net.
	Zero	Zeroes the balance.  The balance must always be zeroed before starting the weighing process. After zeroing, the balance sets a new zero point.
	Home	To return from any menu level to the main weighing screen.

### 3.5 Overview interface connections

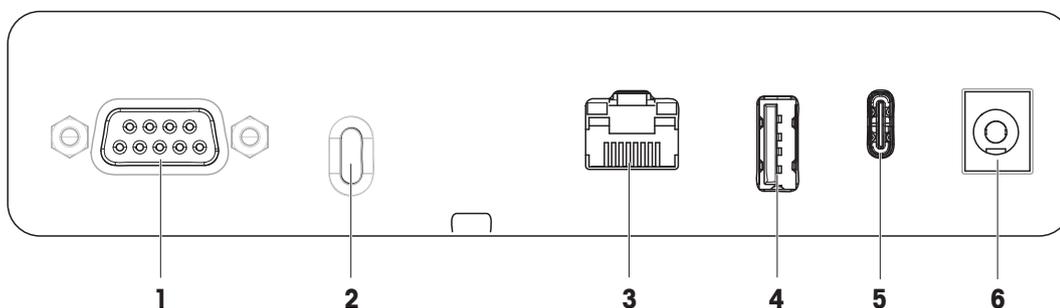


<b>1</b>	RS232C serial interface	<b>4</b>	USB-A port
<b>2</b>	Slot for anti-theft cable	<b>5</b>	USB-C port
<b>3</b>	Ethernet port (LAN)	<b>6</b>	Socket for AC/DC adapter

## 3.6 Components description


### 3.6.1 Draft shield

The draft shield protects the weighing area against environmental impacts like drafts or moisture. The side doors and the top door can be opened manually.

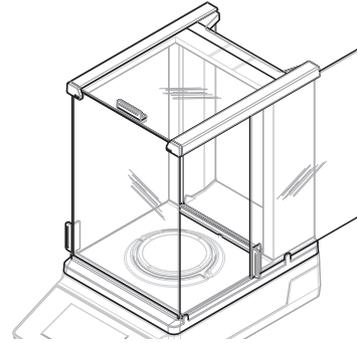


### 3.6.2 Weighing pan

The weighing pan is the load receptor that serves to accommodate the weighing item.

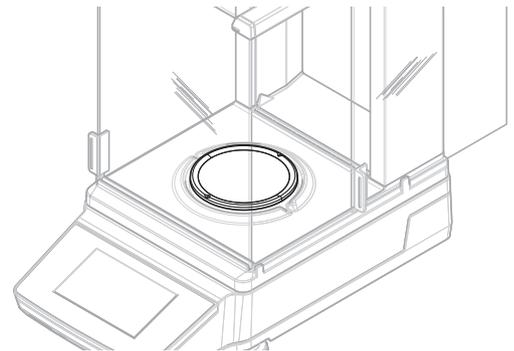


### 3.6.3 Drip tray

The drip tray is positioned below the weighing pan. The primary purpose of the drip tray is to ensure quick cleaning of the balance.

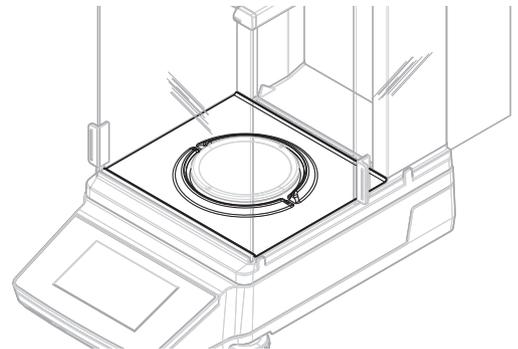


### 3.6.4 Door handle

The door handles are mounted on the draft shield doors. The handles are used to manually open the side doors and the top door of the draft shield.

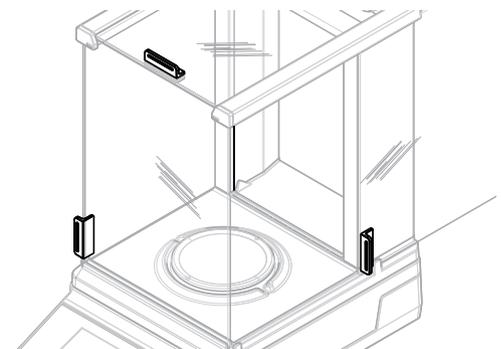


### 3.6.5 Leveling feet

The balance stands on height-adjustable feet. These feet are used to level the balance.

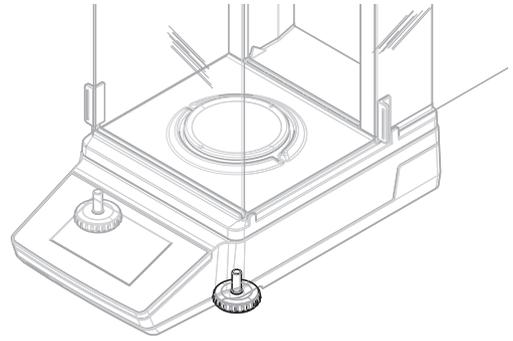


### 3.6.6 Terminal

The balance terminal has a 4.3-inch touch-sensitive display. The terminal and the weighing platform are protected by a replaceable cover.

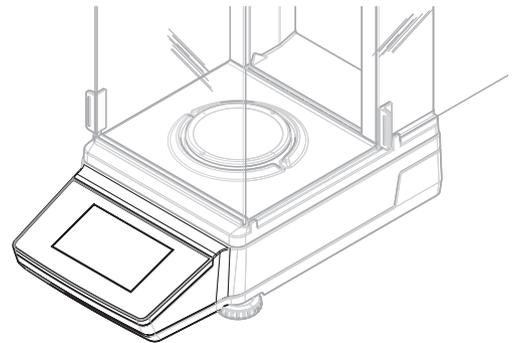


### 3.6.7 QuickLock for draft shield

The QuickLock for the draft shield is used to secure the draft shield to the weighing platform.

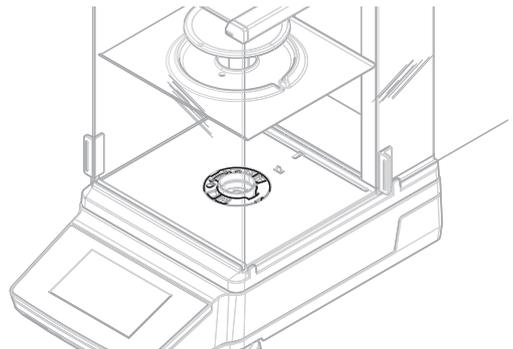


### 3.6.8 QuickLock for doors and front panel

Depending on the position, the QuickLock is used to lock/unlock the top door, the side doors, and the front panel of the draft shield.

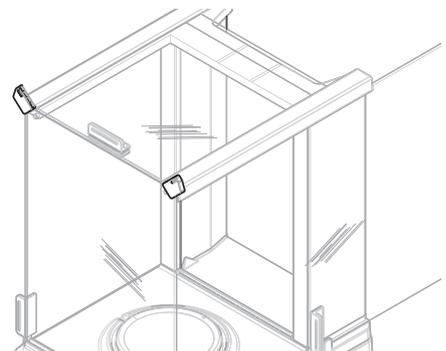

### 3.6.9 Release button for back panel

The release button is used to lock/unlock the back panel of the draft shield.

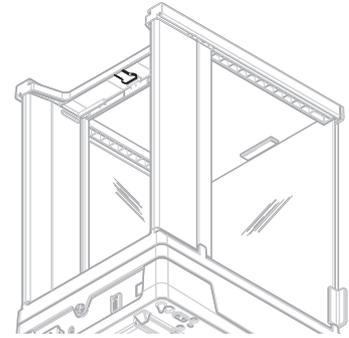

### 3.7 Overview type label

The information on the type label helps to identify the balance.




<b>1</b>	Balance model	<b>5</b>	Manufacturer
<b>2</b>	Year of manufacture	<b>6</b>	Balance serial number
<b>3</b>	Maximum capacity	<b>7</b>	Power consumption
<b>4</b>	Readability		

## 3.8 User interface

### 3.8.1 Main sections at a glance

The main weighing screen (1) is the central navigation point where all the menus and settings can be found. The sections **Balance menu** (2), **Main configuration** (3), and the applications section (4) open when tapping the corresponding icon or tab.

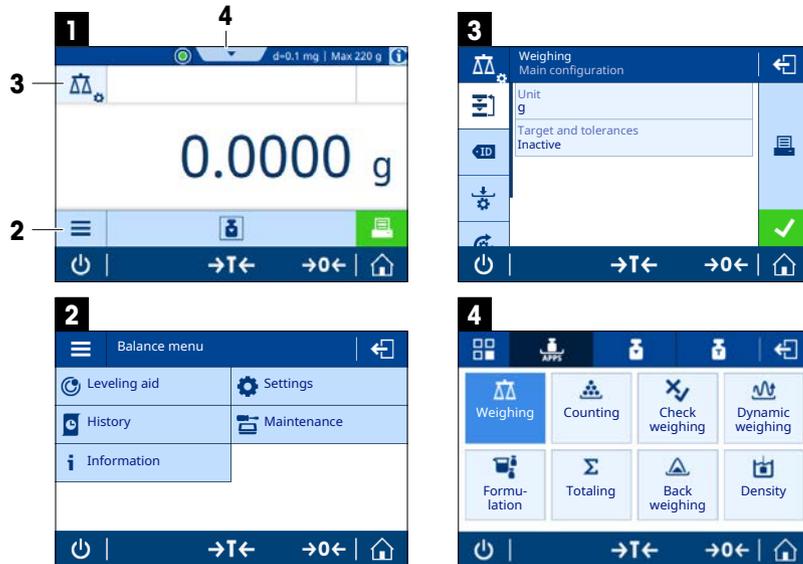

#### See also

- [Main weighing screen](#) ▶ Page 18
- [Balance menu](#) ▶ Page 19
- [Main configuration](#) ▶ Page 20
- [Applications](#) ▶ Page 20


### 3.8.2 Main weighing screen



	Name	Description
1	Weighing results	Shows the results of the current weighing process.
2	Level indicator	Indicates if the balance is leveled (green) or not (red).


	Name	Description
3	Applications	Accesses available applications: <b>Weighing, Adjustments, Tests.</b>
4	Readability and capacity	Shows the readability and the capacity of the balance.
5	Additional information	Shows additional information about the current activity. Example: current weighing value in another unit
6	Information and warnings	Shows current information, warnings, and error messages.
7	Functions area	Shows the active functions according to the settings of the current weighing application.
8	<b>Publish</b> button	Publishes the results according to the settings of the current weighing application. Depending on the selected weighing application, the button can have different functions.
9	Action bar	Contains actions referring to the current weighing application.
10	<b>Balance menu</b>	Accesses the balance properties.
11	SmartTrac	Used as a weighing aid to define a target weight with upper and lower tolerances.
12	<b>Main configuration</b>	Accesses the configuration options for the current weighing application.

### 3.8.3 Balance menu

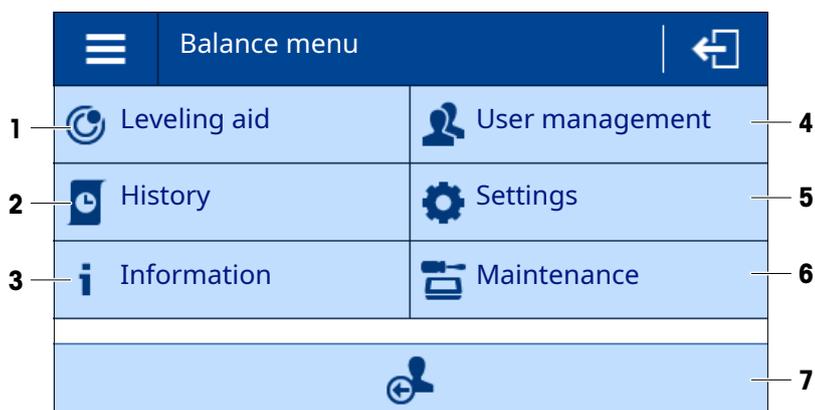


	Name	Description
1	<b>Leveling aid</b>	Opens the leveling dialog.
2	<b>History</b>	Opens the history dialog.
3	<b>Information</b>	Opens the balance information.
4	<b>User management</b>	Opens the user management dialog (only visible if activated).
5	<b>Settings</b>	Opens the settings dialog.
6	<b>Maintenance</b>	Opens the maintenance dialog.
7	Logout	Function related to the menu topic <b>User management.</b>

### 3.8.4 Main configuration

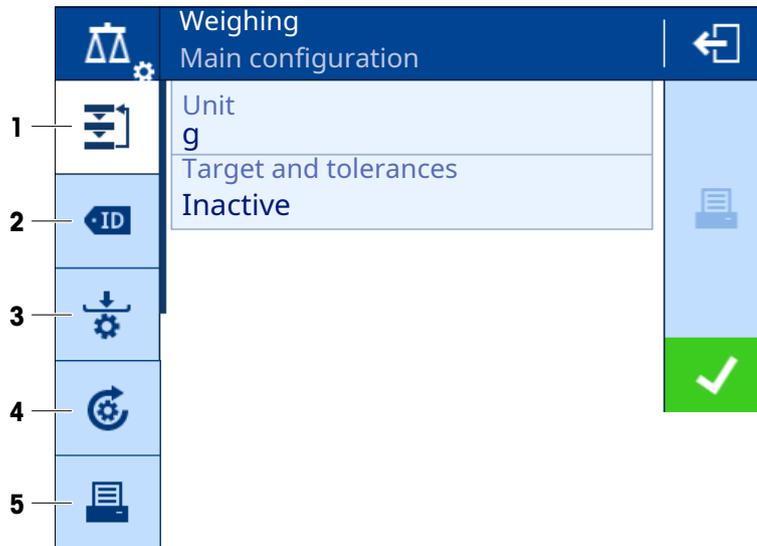

	Name	Description
1	<b>Main configuration</b>	Opens the main configuration.
2	<b>ID format</b>	Opens the sample ID configuration.
3	<b>Weighing configuration</b>	Opens the weighing configuration.
4	<b>Automation</b>	Opens the automation configuration.
5	<b>Report configuration</b>	Opens the report configuration.

### 3.8.5 Applications

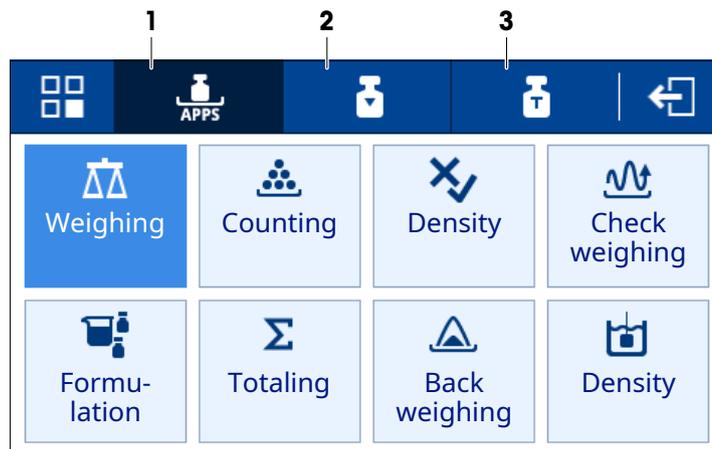

	Name	Description
1	<b>Weighing</b>	Contains available weighing applications.
2	<b>Adjustments</b>	Contains available adjustments.
3	<b>Tests</b>	Contains available tests.

### 3.8.6 Icons and symbols

#### 3.8.6.1 System status icons

System messages appear due to a user action, a user input, or a system process. When tapping the icon, the corresponding system message is displayed.

Icon	Name	Description
	Levelled	Indicates that the balance is correctly levelled.
	Not levelled	Indicates that the balance is not levelled.
	<b>Information</b>	Provides information related to the current action or process.
	Warning	Provides information about an issue that requires attention.
	Error	Provides information about a failed action or process.

#### 3.8.6.2 Weighing status icons

Icon	Name	Description
	Stability indicator	Indicates that the weighing process is ongoing. The weighing result is not yet stable.
<b>Net</b>	Net indicator	Appears when pressing the tare key, after the tare weight has been subtracted.
	Calculated value	The current weight value is calculated.
	Minimum weight violation	The current weight value is smaller than the defined minimum weight. The weight must be larger than the minimum weight.

#### 3.8.6.3 Process status icons

Icon	Name	Description
	<b>Start</b>	Starts the process.
	<b>Pause</b>	Pauses the process
	<b>Continue</b>	Continues a paused process.
	<b>Add</b>	Adds the displayed result to a measurement series.

Icon	Name	Description
	<b>Complete</b>	Completes the process.
	<b>Stop</b>	Stops the process.

## 4 Installation and Putting into Operation

### 4.1 Selecting the location

A balance is a sensitive precision instrument. The location where it is placed will have a profound effect on the accuracy of the weighing results.

#### Requirements of the location

Place indoors on stable table


Ensure sufficient spacing

Level the instrument

Provide adequate lighting




Avoid direct sunlight



Avoid vibrations



Avoid strong drafts



Avoid temperature fluctuations



Take into account the environmental conditions. See "Technical Data".

Sufficient spacing for balances: > 15 cm all around the instrument


### 4.2 Unpacking the balance

Check the package, the packaging elements and the delivered components for damages. If any components are damaged, please contact your METTLER TOLEDO service representative.


#### **i** Note

Depending on the balance model, the packaging elements and the components may look different.


- 1 Open the box and lift the package out using the lifting strap **(1)**.
- 2 Place the package on a level surface with the inscription **BOTTOM (2)** facing downwards.

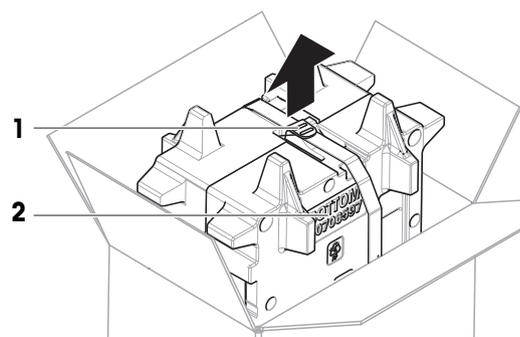


- 3 Open the lifting strap (1) and remove the User Manual (3).

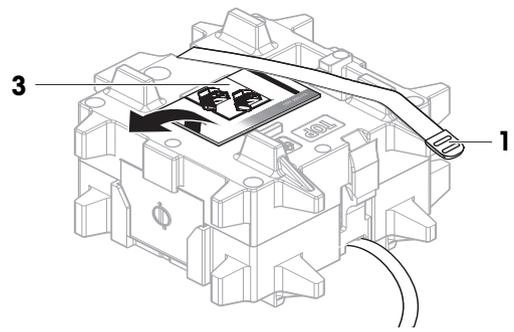

- 4 Remove the upper part of the package and unpack the drip tray (4).

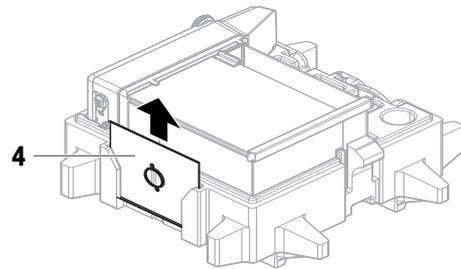

- 5 Carefully unpack the balance (5) and all other items.
- 6 Remove the protective bag.
- 7 Keep the protective cover installed on the weighing platform and on the terminal.
- 8 Store all parts of the packaging in a safe place for future use.
  - ➔ The balance is ready for installation.

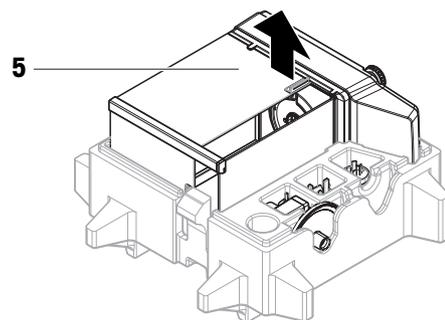

## 4.3 Installation

### Note

Depending on the balance model, the components may look different.

### 4.3.1 Balances with draft shield



#### CAUTION

##### **Injury due to sharp objects or broken glass**


Instrument components, e.g., glass, can break and lead to injuries.

- Always proceed with focus and care.


### Note

Skip steps 1 – 4 when unpacking the balance for the first time, or if the draft shield is already assembled.


- 1 Assemble the draft shield: Turn the QuickLock (**1**, right, left) and slide in the top door (**2**).

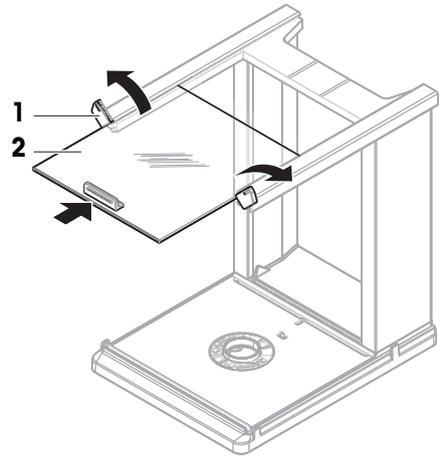


- 2 Slide in the side door (**3**) (right, left).

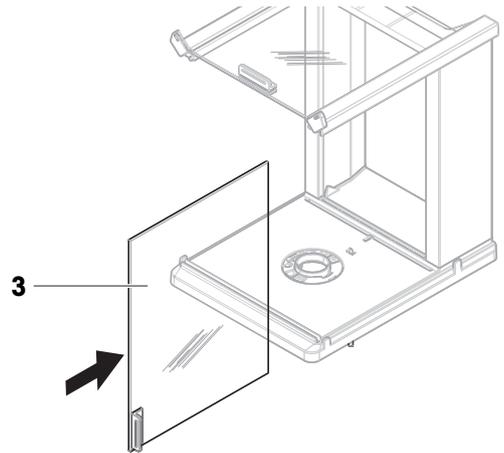

- 3 Attach the front panel (**4**), then turn the QuickLock (**1**, right, left) to hold the panel in place.

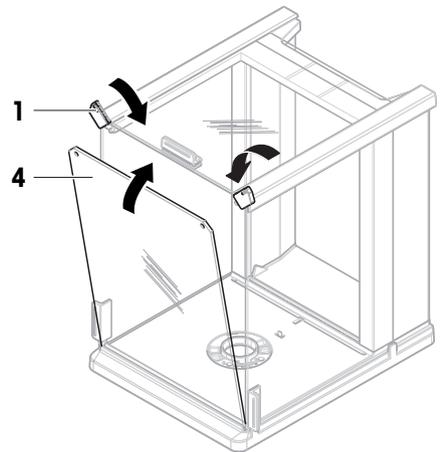


- 4 Attach the back panel (5). Make sure the release button (6) snaps in.  
➔ The draft shield is assembled.

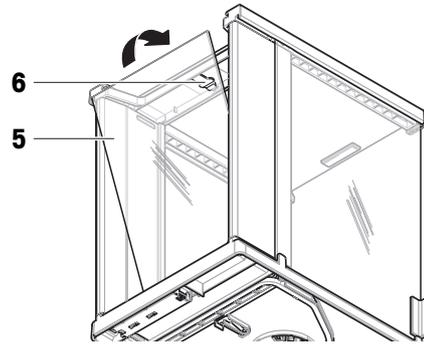


- 5 Secure the draft shield (7) to the weighing platform (9) by turning the QuickLock (8).

**Note**

To protect your balance, keep the protective cover installed on the weighing platform (9).

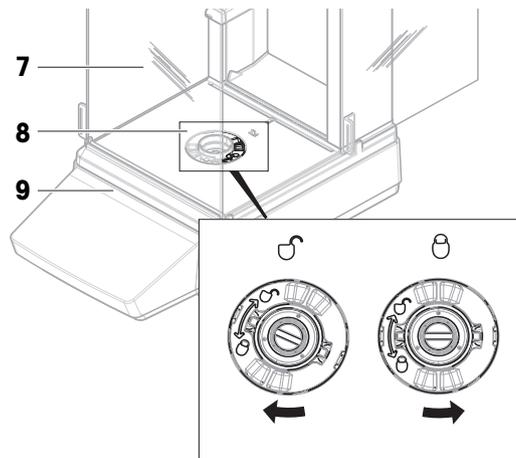


- 6 Insert the drip tray (10).

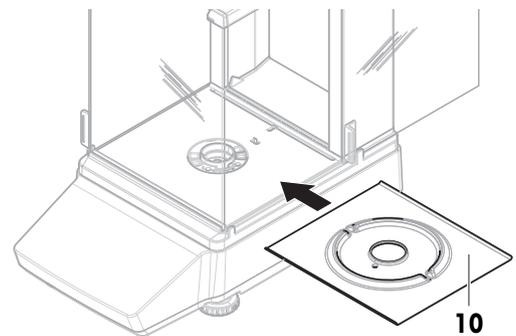

- 7 Install the weighing pan (11).

➔ The balance is ready for use.

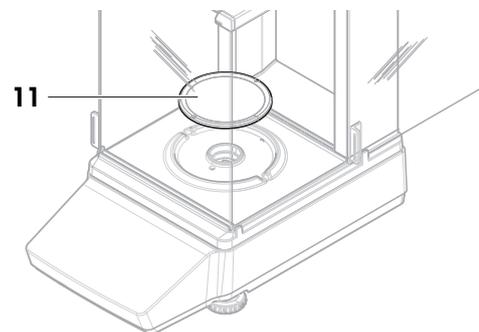


### 4.3.2 Balances without draft shield

- 1 Place the draft-protection element (1) on top of the weighing platform (2).

**Note**

To protect your balance, keep the protective cover installed on the weighing platform (2).

- 2 Place the weighing pan support (3) on top of the weighing platform (2).
- 3 Place the weighing pan (4) on the weighing pan support (3).  
➔ The balance is ready for use.

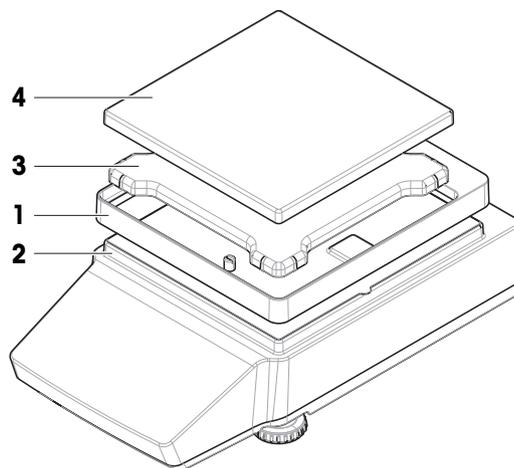

## 4.4 Putting into operation

### 4.4.1 Connecting the balance




#### **WARNING**

##### **Death or serious injury due to electric shock**

Contact with parts that carry a live current can lead to death or injury.

- 1 Only use the METTLER TOLEDO power cable and AC/DC adapter designed for your instrument.
- 2 Connect the power cable to a grounded power outlet.
- 3 Keep all electrical cables and connections away from liquids and moisture.
- 4 Check the cables and the power plug for damage and replace them if damaged.

- 1 Install the cables in such a way that they cannot be damaged or interfere with operation.
- 2 Insert the plug of the AC/DC adapter (1) into the power socket of the instrument.
- 3 Insert the plug of the power cable into a grounded power outlet that is easily accessible.  
➔ The balance automatically switches on.

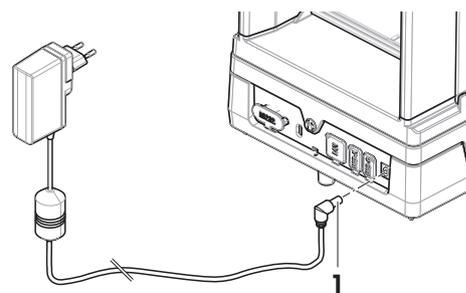

**Note**

Do not connect the instrument to a power outlet controlled by a switch. After switching on the instrument, it must warm up before giving accurate results.

#### **See also**

[General data](#) ▶ Page 111

## 4.4.2 Switching on the balance

When connected to the power supply, the balance automatically switches on.

### EULA (End User License Agreement)

When the balance is switched on the first time, the EULA (End User License Agreement) appears on the screen.

- 1 Read the conditions.
- 2 Tap **I accept the terms in the license agreement** and confirm with **✓ OK**.
  - ➔ The main weighing screen appears.

### Acclimatization and warm up

Before the balance gives reliable results, it must:

- acclimatize to the room temperature
- warm up by being connected to the power supply

The acclimatization time and warm-up time for balances are available in "General data".

### Note

When the balance is exiting standby, it is ready immediately.

### See also

-  General data ▶ Page 111
-  Entering / Exiting standby mode ▶ Page 29
-  Entering / Exiting power-saving mode ▶ Page 29
-  Switching off the balance ▶ Page 29

## 4.4.3 Leveling the balance


Exact horizontal and stable positioning are essential for repeatable and accurate weighing results.

If the balance is out of level, the level indicator on the main screen turns red.

- 1 On the main weighing screen, tap .
  - ➔ The dialog **Leveling aid** opens.
- 2 Turn both leveling feet **(1)** as instructed on the display until the dot is in the center of the level indicator.

Alternative access to the dialog **Leveling aid**:

**≡ Navigation: ≡ Balance menu >  Leveling aid**

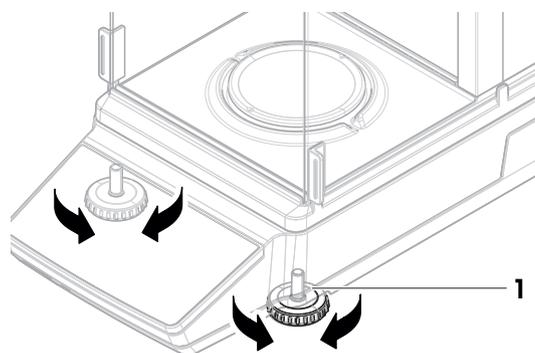

## 4.4.4 Performing an internal adjustment

**≡ Navigation: ▼ >  Applications >  Adjustments**

■ **Adjustments** is set to **Internal**.

- 1 Option 1: On the main weighing screen, tap  **Adjust**.  
Option 2: Open the applications section, tap  **Adjustments**, select the adjustment, and tap **▶ Start**.
  - ➔ The adjustment is executed.
  - ➔ The adjustment results appear.
- 2 Tap **✓ Finish**.
  - ➔ The balance is ready.

#### 4.4.5 Entering / Exiting standby mode

- 1 To enter standby mode, short press 
  - ➔ The display is blue. A QR code for more information about the balance is shown.
- 2 To exit standby mode, short press 
  - ➔ The display is turned on.

#### 4.4.6 Entering / Exiting power-saving mode

- 1 To enter power-saving mode, long press  (more than two seconds).
  - ➔ The display is dark. The balance is in power-saving mode.
- 2 To exit power-saving mode, long press 
  - ➔ The balance is switched on.

##### **Note**

We recommend configuring power-saving times. When the balance exits power-saving mode automatically at the defined time, the balance is ready for use immediately.

If the power-saving mode is terminated manually, the balance must warm up before it can be used.

##### **See also**

-  General data ▶ Page 111
-  Standby, Power-saving mode ▶ Page 34

#### 4.4.7 Switching off the balance

To completely switch off the balance, it must be disconnected from the power supply. By pressing , the balance goes only into standby mode or into power-saving mode.

##### **Note**

When the balance has been completely switched off for some time, it must warm up before it can be used.

##### **See also**

-  Switching on the balance ▶ Page 28
-  Entering / Exiting standby mode ▶ Page 29
-  Entering / Exiting power-saving mode ▶ Page 29


### 4.5 Performing a simple weighing

##### **Note**

A balance with draft shield is used to explain the procedure. For balances without a draft shield, skip the instructions steps concerning the draft shield.

#### 4.5.1 Opening and closing draft shield doors

- Open the door manually with the door handle (1).

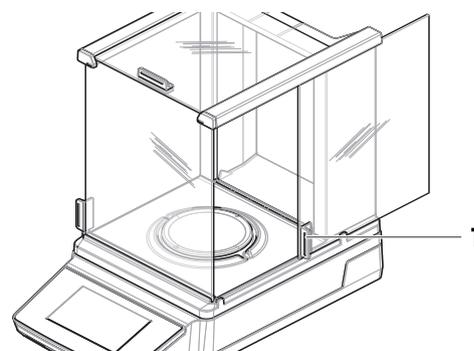


## 4.5.2 Zeroing the balance

- 1 Open the draft shield.
- 2 Clear the weighing pan.
- 3 Close the draft shield.
- 4 Press **→0←** to zero the balance.
  - ➔ The balance is zeroed.

## 4.5.3 Taring the balance

If a sample vessel is used, the balance must be tared.

- The balance is zeroed.
- 1 Place the sample vessel (1) on the weighing pan (2).
  - 2 Press **→T←** to tare the balance.
    - ➔ The balance is tared. The icon **Net** appears.

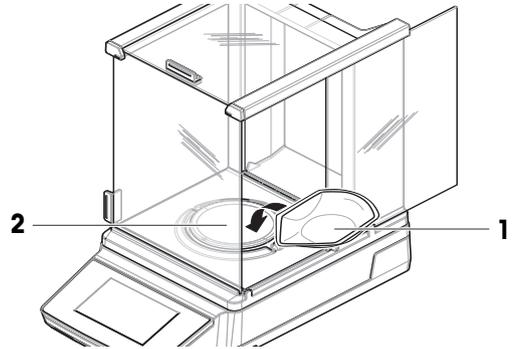

## 4.5.4 Performing a weighing

- 1 Open the draft shield.
- 2 Place the weighing object into the sample vessel.
- 3 Close the draft shield.
  - ➔ The result is displayed.
- 4 Optional, if a printer is connected: Tap  to print the weighing result.


## 4.6 Transporting, packing, and storing

### 4.6.1 Transporting the balance over short distances

- 1 Disconnect the AC/DC adapter and unplug all interface cables.
- 2 Hold the balance with both hands and carry it in horizontal position to the target location. Consider the requirements of the location.

If you want to put the balance into operation, proceed as follows:

- 1 Connect in reverse order.
- 2 Give the balance sufficient time to warm up.
- 3 Level the balance.
- 4 Perform an internal adjustment.

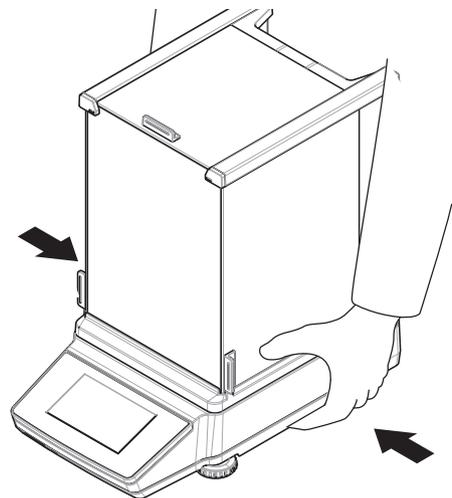

### See also

- 🔗 Selecting the location ▶ Page 23
- 🔗 Switching on the balance ▶ Page 28
- 🔗 Leveling the balance ▶ Page 28
- 🔗 Performing an internal adjustment ▶ Page 28

## 4.6.2 Transporting the balance over long distances

METTLER TOLEDO recommends using the original packaging for transportation or shipment of the balance or balance components over long distances. The elements of the original packaging are developed specifically for the balance and its components and ensure maximum protection during transportation.

### See also

- 🔗 Unpacking the balance ▶ Page 23

## 4.6.3 Packing and storing

### Packing the balance

Store all parts of packaging in a safe place. The elements of the original packaging are developed specifically for the balance and its components, and ensures maximum protection during transportation and storage.

### Storing the balance

Only store the balance under the following conditions:

- Indoor and in the original packaging
- According to the environmental conditions, see "Technical Data"

### **i** Note

When storing for longer than 6 months, the rechargeable battery may become empty (only date and time get lost).

### See also

- 🔗 Technical Data ▶ Page 111

## 4.7 Weighing below the balance

Your balance is equipped with a weighing hook for performing weighing operations below the work surface (weighing below the balance).

- A weighing table or workbench is available, through which the weighing hook can be accessed.

- 1 Disconnect the balance from the AC/DC adapter.
- 2 Disconnect all interface cables.
- 3 Carefully tilt the balance to its side.
- 4 Remove the weighing hook cover (1).


### **i** Note

Except for balance model MR304, the weighing hook is located closer to the front.

- ➔ The hook (2) is accessible.

- 5 Carefully put the balance back on its feet.
- 6 Reconnect the AC/DC adapter and the interface cables.

- ➔ The weighing hook is accessible and can be used for below-the-balance weighing.

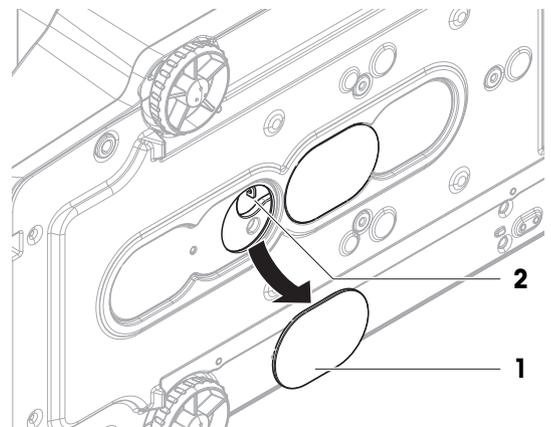

### See also


- 🔗 Dimensions ▶ Page 116

## 5 Operation

### 5.1 Touchscreen


#### 5.1.1 Selecting or activating an item

1. Tap the item or function you want to select or activate.

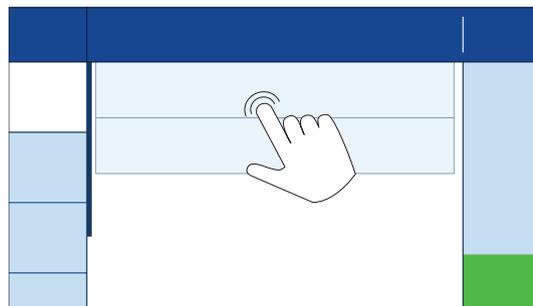


#### 5.1.2 Scrolling

1. Scroll up or down to view all items.

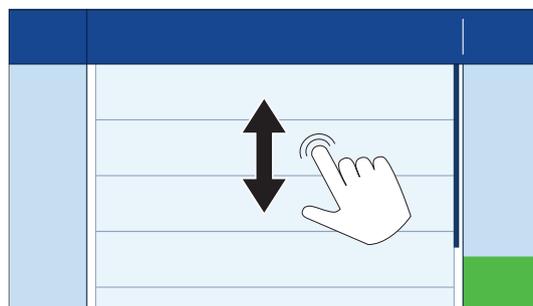

#### 5.1.3 Opening the fly-in panel


1. Tap the tab, or pull the tab down, to open the fly-in panel.

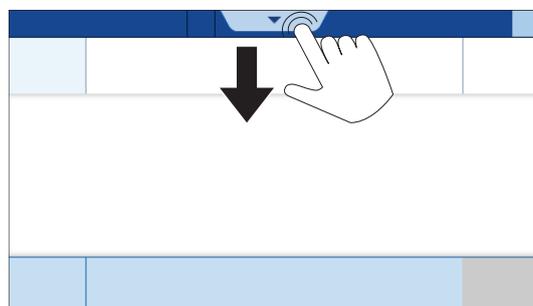

#### 5.1.4 Entering characters and numbers


**Note**

Tapping and holding a character gives access to special characters.

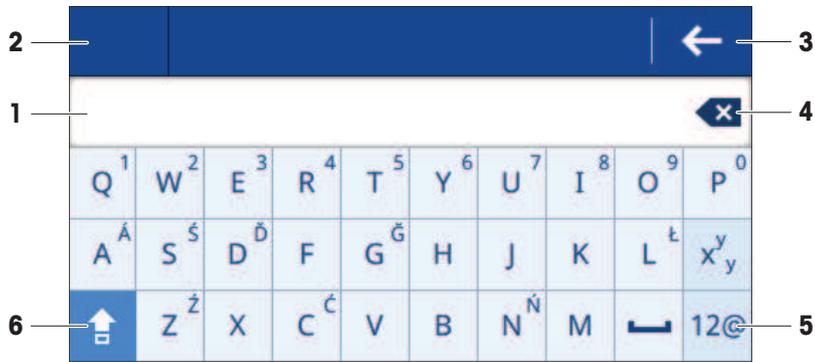


	Name	Description
1	Input field	Shows the entered characters and numbers.
2	Section title	Shows the icon and the title of the current section.
3	Back	Closes the keyboard dialog.
4	Backspace	A short press deletes the last character of the entry. A long press deletes the whole entry.
5	Numbers and special characters	Allows to enter special characters.
6	Shift	Switches between lowercase and uppercase.

### 5.1.5 Changing values

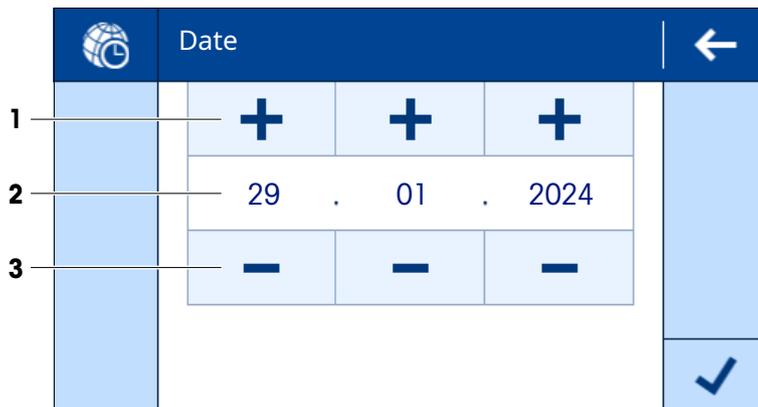

	Name	Description
1	Plus button	Increases the value.
2	Value field	Shows the defined value.
3	Minus button	Decreases the value.

## 5.1.6 Sliding

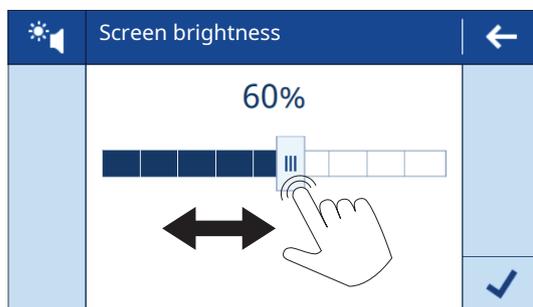

- Move the slider left or right to change the value.

## 5.2 General balance settings

### 5.2.1 Date / Time / Language

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > 🕒 **Date / Time / Language**

- The setting **Date / Time / Language** is open.
  - 1 Optional: Tap the settings **Date format** and **Time format** to define how date and time are displayed.
  - 2 Tap the setting **Date** to adjust the date.
  - 3 Tap ✓ **OK**.
  - 4 Tap the setting **Time** to adjust the time.
  - 5 Tap ✓ **OK**.
  - 6 Tap the setting **Language** and select the system language of your choice.
  - 7 Tap ✓ **OK**.
  - 8 Tap ✓ **Save**.

#### **Note**

The internal clock can show a time deviation. Adjust the time if necessary.

#### **See also**

🔗 [Settings: Date / Time / Language ▶ Page 73](#)

### 5.2.2 Screen / Sound

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > 🔊 **Screen / Sound**

- The setting **Screen / Sound** is open.
  - 1 Tap the setting **Screen brightness** to adjust the brightness of the display.
  - 2 Tap ✓ **OK**.
  - 3 Tap the setting **Sound volume** to adjust the volume level.
  - 4 Tap ✓ **OK**.

#### **See also**

🔗 [Settings: Screen / Sound ▶ Page 73](#)

### 5.2.3 Standby, Power-saving mode

The function **Standby** helps to save power consumption during the working hours. Outside of the working hours, the function **Power-saving mode** serves to hibernate the balance.

When the balance is switched on from status **Standby**, it is ready for use immediately. When switched on from status **Power-saving mode**, the balance must warm up before use.

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > ⚙️ **General**

■ The setting **General** is open.

1 Tap the setting **Standby**.

**Note**

This function can be activated or deactivated.

2 Enter the time after which the balance goes into standby.

3 Tap ✓ **OK**.

4 Tap the setting **Power-saving mode**.

**Note**

This function can be activated or deactivated.

5 Define the settings **Start work** and **End work**.

**Note**

When the balance exits power-saving mode automatically at the defined time, the balance is ready for use immediately.

6 Select the working days.

**Note**

During the defined time, the function **Power-saving mode** is not used.

7 Tap ✓ **OK**.

8 Tap ✓ **Save**.

**See also**

🔗 [Settings: General](#) ▶ Page 74

## 5.2.4 Weighing / Quality

### 5.2.4.1 Warnings and reminders

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > ⚖️ **Weighing / Quality**

#### Leveling warning

Typically, the leveling is done when required. If the option **Forced leveling** is selected, the balance must be leveled before it can be used.

■ The setting **Weighing / Quality** is open.

1 Tap the setting **Leveling warning**.

**Note**

This function can be activated or deactivated.

2 Select the option of your choice.

3 Tap ✓ **OK**.

**See also**

🔗 [Settings: Weighing / Quality](#) ▶ Page 70

### 5.2.4.2 Weighing profiles

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > ⚖️ **Weighing / Quality** > ⚖️ **Weighing profiles**

A weighing profile serves to adapt the balance to specific requirements. Up to three weighing profiles can be defined.

**See also**

🔗 [Settings: Weighing / Quality](#) ▶ Page 70

### 5.2.4.2.1 Environment

This setting serves to adapt the balance to the ambient conditions of a specific location.

- The setting **Weighing profiles** is open.
- 1 Enter a name for the profile.
- 2 Tap the setting **Environment**.
- 3 Select the option that fits the environmental condition.
- 4 Tap ✓ **OK**.

#### See also

 Settings: Weighing / Quality ▶ Page 70

### 5.2.4.2.2 Weighing mode

This setting defines how weighing signals are filtered. For standard weighing applications, the option **Universal** is appropriate.

- The setting **Weighing profiles** is open.
- 1 Tap the setting **Weighing mode**.
- 2 Select the option that fits your needs.
- 3 Tap ✓ **OK**.

### 5.2.4.2.3 Value release

This setting defines how quickly a weighing result is considered stable.

- The setting **Weighing profiles** is open.
- 1 Tap the setting **Value release**.
- 2 Select the option that fits your needs.
- 3 Tap ✓ **OK**.

#### See also

 Settings: Weighing / Quality ▶ Page 70

## 5.3 Weighing applications

A weighing application serves to carry out specific weighing tasks. The balance offers various weighing applications with default parameters.

### 5.3.1 Weighing applications overview

The section **Weighing** provides an overview of weighing applications available on the balance. This section serves to select a weighing application for a specific weighing procedure.

☰ **Navigation:** ▼ >  **Applications** > 

The following weighing applications are available:

-  **Weighing**
-  **Counting**
-  **Check weighing**
-  **Dynamic weighing**
-  **Formulation**
-  **Totaling**
-  **Back weighing**
-  **Density**

## 5.3.2 General settings for weighing applications

### 5.3.2.1 Defining target weight and tolerances

Some weighing applications provide the option to define a target weight. You can also define a tolerance range for the weighing result. Instead of a  $\pm$  tolerance range, you can define an upper (+) and/or a lower (-) tolerance limit. If the weighing result is out of range, this is indicated on the main weighing screen.

☰ **Navigation:** ▼ >  >  **Weighing** > 

This example shows how to define a target weight and a tolerance range for the application **Weighing**. The procedure for other weighing applications is similar.

- The section  **Main** is open.
- 1 Tap the setting **Target and tolerances**.
  -  **Note**  
This function can be activated or deactivated.
  - ➔ The section  **Target** is open.
- 2 Enter a target weight.  
Alternatively, tap  to define the target value with an actual weight.
- 3 Tap   **± Tol..**
  -  **Note**  
This function can be activated or deactivated.
- 4 Enter a tolerance range [% or unit].
  -  **Note**  
Tap the corresponding icon to switch between % and unit.
- 5 Tap  **OK**.
- 6 Tap  **Save**.
  - ➔ The target weight and the tolerance range are shown on the main weighing screen.
  -  **Note**  
Due to limited space on the display, these values are always shown in percentage [%]. This also applies if you configured this setting to use a unit.

#### See also

 [Main configuration](#) ▶ Page 77

### 5.3.2.2 Defining a sample ID

☰ **Navigation:** ▼ >  >  **Weighing** > 

This example shows how to define a sample ID for the application **Weighing**. The procedure for other weighing applications is similar.

- The settings section of the weighing application is open.
- 1 Tap  **ID format**.
- 2 Tap **Sample ID**.
  -  **Note**  
This function can be activated or deactivated.
- 3 Tap **Default value** and enter a value.
- 4 Tap  **OK**.

### Adding a description

You can add up to three descriptions to a sample.

- The section  **ID format** is open.
- 1 Tap **Description 1**.
  -  **Note**  
This function can be activated or deactivated.
- 2 Tap **Type** and select the option **Sample**.
- 3 Tap **Label** to enter a description.
- 4 Tap  **OK**.
- 5 Tap **Default value** to enter a value.
- 6 Tap  **OK**.
- 7 Tap **Input prompt**. If this option is activated, you are prompted to enter a value for the sample ID.
- 8 Tap  **OK**.
- 9 Tap  **Save**.

### 5.3.2.3 Configuring a weighing application

≡ **Navigation:**  **Weighing** > 

This example shows how to configure the application **Weighing**. The procedure for other weighing applications is similar.

- The settings section of the weighing application is open.
- 1 Tap  **Weighing**.
- 2 Tap **Info weight** and select a unit for the secondary weight to be displayed on the main weighing screen.
  -  **Note**  
This function can be activated or deactivated.
- 3 Tap **Weighing profile** and select the option of your choice.
- 4 Tap  **OK**.
- 5 Tap **Weight capture mode** and select the option of your choice.
- 6 Tap  **Save**.

#### See also

 Weighing configuration ▶ Page 78

### 5.3.2.4 Configuring a weighing series

Some weighing applications provide the option to define a weighing series. If this option is activated, the balance can also provide statistical calculations.

≡ **Navigation:**  **Weighing** > 

This example shows how to configure a weighing series for the application **Weighing**. The procedure for other weighing applications is similar.

- The settings section of the weighing application is open.
- 1 Optional, if activated: Tap  **ID format**, then tap **Description**.
- 2 Tap **Type** and select the option **Series**.
- 3 Tap  **OK**.
- 4 Tap Automatic value if you want to activate an automatic timestamp.
  -  **Note**  
If activated, this setting deactivates the options **Default value** and **Input prompt**.
- 5 Tap  **OK**.
- 6 Tap  **Weighing**.

- 7 Tap **Measurement series** to activate this function.
- 8 Optional: Tap **Statistical calculations** to activate this function.
- 9 Optional: Tap **Acceptance range** and enter a value.

**Note**

This function can be activated or deactivated.

- 10 Tap **✓ OK**.
- 11 Tap **✓ Save**.

**See also**

[Weighing configuration](#) ▶ Page 78

### 5.3.2.5 Using automated functions

Most weighing applications provide the option to automate specific functions. For example, with the option **Automatic tare**, the balance automatically stores the first stable weight as the tare weight.

☰ **Navigation:** ▼ >  >  **Weighing** > 

This example shows how to select automated functions for the application **Weighing**. All functions can be activated or deactivated individually. The procedure for other weighing applications is similar.

- The section  **Automation** is open.
- 1 Tap **Automatic zero** and enter a threshold below which the balance is automatically zeroed.

**Note**

Select the unit of your choice.

- 2 Tap **✓ OK**.
- 3 Tap **Automatic tare** to activate or deactivate this function.
- 4 Tap **Recall weight** and select the option of your choice.
- 5 Tap **✓ OK**.
- 6 Tap **✓ Save**.
  - ➔ The main weighing screen opens.
- 7 Tap .
- 8 Enter a preset tare weight.
- 9 Tap **✓ Apply**.
  - ➔ The preset tare weight is shown on the main weighing screen.

**See also**

[Automation](#) ▶ Page 79

### 5.3.2.6 Configuring a report

By default, only the weighing result and the weight unit are published. The report can be configured to show more information. The report defines the content for the following publishing strategies:

- printing data on a printer
- exporting data to a file on a USB storage device
- transferring data to the software **EasyDirect Balance**

☰ **Navigation:** ▼ >  >  **Weighing** > 

This example shows how to configure a report for the application **Weighing**. The procedure for other weighing applications is similar.

- The settings section of the weighing application is open.
- 1 Tap  **Report**.
  - 2 Tap **Header and Footer**.
  - 3 Tap the items you want to have in the report.

- 4 Tap **Title** to enter a title name.
- 5 Tap ✓ **OK**.
- 6 Tap **Empty lines** and enter a number.
- 7 Tap ✓ **OK**.
- 8 Tap > to get to the next section of the report configuration.
- 9 Tap the items you want to have in the report.
- 10 Continue until you have reached the last section of the report configuration.
- 11 Tap ✓ **Save**.

**See also**

🔗 Report configuration ▶ Page 79

### 5.3.3 Application "Weighing"


The application **Weighing** offers basic weighing functions. This application is used for simple weighing tasks, or to perform a measurement series.

The settings of the weighing item, such as target weight and tolerances, can be specified.

☰ **Navigation:** ▼ >  >  **Weighing**

**Example procedure**

- 1 Open the applications section.
  - ➔ The section  is selected.
- 2 Tap  **Weighing**.
  - ➔ The corresponding weighing application opens.
- 3 Press → **0** ← to zero the balance.
- 4 Open the draft shield door (if applicable).
- 5 Place the weighing object (**1**) on the weighing pan (**2**).
- 6 Close the draft shield door (if applicable).
- 7 Wait until the weight stabilizes.
  - ➔ The result is displayed.
- 8 Optional, depending on the settings: Tap  **Publish** to print or export the weighing result.

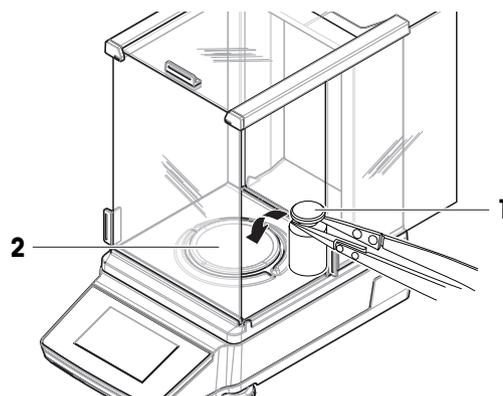

**See also**

🔗 Settings: application "Weighing" ▶ Page 77

### 5.3.4 Application "Counting"

The application **Counting** is used to determine the number of pieces put on the weighing pan. It is advantageous if all pieces are of approximately equal weight, since the unit quantity is determined on the basis of the average weight of a defined number of reference pieces.

☰ **Navigation:** ▼ >  >  **Counting**

**Example procedure**

This example shows how to weigh pieces in a sample vessel.

- 1 Open the applications section.

- ➔ The section  is selected.
- 2 Tap  **Counting**.
  - ➔ The corresponding weighing application opens.
- 3 Tap the title section **Reference**.  
Alternatively, tap  to access this setting.
  - ➔ The screen to define the reference weight opens.
- 4 Tap on the left title section to define the number of reference pieces. For example, enter 5.
- 5 Tap **✓ OK**.
- 6 Place an empty sample vessel on the weighing pan.
- 7 Press **→T←** to tare the balance.
- 8 Put the five reference pieces into the sample vessel.
  - ➔ The total weight of the reference pieces is displayed.
- 9 Tap **✓ OK**.
  - ➔ The number of reference pieces is indicated.
  - ➔ The weight of one reference piece is displayed in the left title section.
- 10 Add pieces to the sample vessel.
  - ➔ The total number of pieces in the sample vessel is displayed.

**See also**

 Settings: application "Counting" ▶ Page 79

### 5.3.5 Application "Check weighing"

The application **Check weighing** checks the deviation of a sample weight within a tolerance limit against a reference target weight.

**Navigation:**  ▼ >  >  **Check weighing**

**Example procedure**

This example shows how to check a sample against a target weight. We use a ± tolerance range.

- 1 Open the applications section.
  - ➔ The section  is selected.
- 2 Tap  **Check weighing**.
  - ➔ The corresponding weighing application opens.
- 3 Tap .
  - ➔ The section **Main configuration** opens.
- 4 Tap **Target weight** and enter a value for the reference sample.
 

 **Note**  
Alternatively, tap  to weigh the reference sample.
- 5 Tap  and enter a value for the tolerances.
- 6 Tap **✓ OK**.
  - ➔ The section **Main configuration** opens.
- 7 Tap **Check threshold** and enter a value.
- 8 Tap **✓ OK**.
  - ➔ The section **Main configuration** opens.
- 9 Tap **✓ Save**.
  - ➔ The main weighing screen opens.
- 10 Place the sample on the weighing pan.
  - ➔ The result is displayed.

**Note**

If the result is within the tolerance range, the background appears green.



If the result is outside the tolerance range, the background appears red.



**See also**

Settings: application "Check weighing" ▶ Page 82

### 5.3.6 Application "Dynamic weighing"

The application **Dynamic weighing** determines the weight of unstable samples. It also allows weighing under unstable ambient conditions. The calculated weight is an average of several weighings over a defined time.

Navigation: ▼ > > **Dynamic weighing**

#### Example procedure

This example shows how to manually start a dynamic weighing in a sample vessel.

- 1 Open the applications section.
  - ➔ The section is selected.
- 2 Tap **Dynamic weighing**.
  - ➔ The corresponding weighing application opens.
- 3 Tap the title section to define the measuring duration in seconds. For example, enter 5.

**Note**

Alternatively, tap to access this setting.

- 4 Tap **OK**.
- 5 Tap **Start mode**.
- 6 Select **Manual**.
- 7 Tap **OK**.
- 8 Tap **Save**.
  - ➔ The main weighing screen opens.
- 9 Place an empty sample vessel on the weighing pan.
- 10 Press to tare the balance.
  - ➔ Net is displayed.
- 11 Place the sample into the sample vessel.
  - ➔ The result is displayed.
- 12 Tap **Start**.
  - ➔ The balance is capturing the dynamic weight for the defined measuring duration.
  - ➔ The result is displayed on a blue background.

13 Tap ✓ **Finish**.

#### See also

🔗 Settings: application "Dynamic weighing" ▶ Page 84

### 5.3.7 Application "Formulation"

The application **Formulation** is used to weigh in multiple components one after the other. The balance displays the total weight of the added components. The function **Fill up** serves to add a component to reach a defined target weight.

☰ **Navigation:** ▼ >  >  **Formulation**

#### Example procedure Formulation

This example shows how to add components to a sample vessel.

- 1 Open the applications section.
  - ➔ The section  is selected.
- 2 Tap  **Formulation**.
  - ➔ The corresponding weighing application opens.
- 3 Press →**0**← to zero the balance.
- 4 Tap ▶ **Start**.
- 5 Place an empty sample vessel on the weighing pan.
- 6 Press →**T**← to tare the balance.
  - ➔ **Net** is displayed.
- 7 Add the first component to the sample vessel.
- 8 Tap **+ Add**.
- 9 Add the second component to the sample vessel.
- 10 Tap **+ Add**.
- 11 Tap  **Complete**.
  - ➔ The result is displayed.

#### Example procedure Fill up

This example shows how to add a liquid to samples to reach a defined target weight.

- 1 Open the applications section.
  - ➔ The section  is selected.
- 2 Tap  **Formulation**.
  - ➔ The corresponding weighing application opens.
- 3 Press →**0**← to zero the balance.
- 4 Tap ▶ **Start**.
- 5 Place an empty sample vessel on the weighing pan.
- 6 Press →**T**← to tare the balance.
  - ➔ **Net** is displayed.
- 7 Place the sample into the sample vessel.
- 8 Tap **+ Add**.
- 9 Place another sample into the sample vessel.
- 10 Tap **+ Add**.
  - ➔ The total weight of the samples is displayed in the title bar.
- 11 Repeat the procedure with all samples.
- 12 Tap  **Fill up**.
  - ➔ The total weight of the samples is displayed.

13 Add liquid to the sample vessel until the desired target weight is displayed.

➔ The weight of the added liquid is displayed in the title section.

14 Tap  **OK**.

15 Tap  **Complete**.

➔ The number of samples and the total weight of the samples is displayed.

#### See also

 Settings: application "Formulation" ▶ Page 86

### 5.3.8 Application "Totaling"

The application **Totaling** is used to separately weigh different samples. The balance automatically calculates the sum of the weighings.

☰ **Navigation:** ▼ >  >  **Totaling**

#### Example procedure

This example shows how to automatically calculate the total weight of separately weighed samples.

1 Open the applications section.

➔ The section  is selected.

2 Tap  **Totaling**.

➔ The corresponding weighing application opens.

3 Press **→0←** to zero the balance.

4 Tap  **Start**.

5 Place the first sample on the weighing pan.

6 Wait until the weight stabilizes.

7 Tap  **Add**.

8 Remove the sample from the weighing pan.

9 Place another sample on the weighing pan.

10 Wait until the weight stabilizes.

11 Tap  **Add**.

➔ The total weight of both samples is displayed in the title section.

12 Remove the sample from the weighing pan.

13 Repeat the procedure for all samples.

14 Tap  **Complete**.

➔ The number of samples and their total weight is displayed.

15 Tap  **Complete**.

#### See also

 Settings: application "Totaling" ▶ Page 88

### 5.3.9 Application "Back weighing"

The application **Back weighing** is used to calculate the difference of two weighing values.

☰ **Navigation:** ▼ >  >  **Back weighing**

#### Example procedure

This example shows how to calculate how much sample remains in a sample vessel after the sample vessel has been emptied.

1 Open the applications section.

➔ The section  is selected.

- 2 Tap **Back weighing**.
  - ➔ The corresponding weighing application opens.
- 3 Tap **Start**.
- 4 Place an empty sample vessel on the weighing pan.
  - ➔ The balance is taring.
- 5 Place the sample into the sample vessel.
  - ➔ **Initial weight**: The weight of the sample is displayed.
- 6 Remove the sample vessel from the weighing pan and remove the sample.
- 7 Place the sample vessel on the weighing pan.
  - ➔ **Final weight**: The weight of the remaining sample is displayed.
  - ➔  $\delta$ : The weight of the removed sample is displayed in the title section.
- 8 Tap **Complete**.
  - ➔ The result is displayed.
- 9 Tap **Finish**.

**See also**

Settings: application "Back weighing" ▶ Page 89

### 5.3.10 Application "Density"

The application **Density** is used to determine the density of solids. Density determination is carried out based on **Archimedes' principle**: A body immersed in a fluid undergoes an apparent loss in weight that is equal to the weight of the fluid it displaces.

**Navigation:** > > **Density**

**Example procedure**

This example describes how to determine the density of a solid with the help of a density kit. A custom auxiliary liquid is used.

- A density kit is available for the balance.
- 1 Open the applications section.
    - ➔ The section is selected.
  - 2 Tap **Density**.
    - ➔ The corresponding weighing application opens.
  - 3 Tap the title section that shows the auxiliary liquid.
 

**Note**  
Alternatively, tap to access this setting.
  - 4 Select **Custom**.
  - 5 Tap **Save**.
  - 6 Tap the title section that shows the density of the auxiliary liquid.
 

**Note**  
Alternatively, tap to access this setting.
  - 7 Enter a value.
 

**Note**  
For water, the density is predefined.
  - 8 Tap **Start**.
  - 9 Place the density kit with the auxiliary liquid on the weighing pan.
  - 10 Tap **OK**.
    - ➔ **Net** is displayed.
  - 11 Place the sample on the weighing pan.

- 12 Tap ✓ **OK**.
- 13 Place the sample into the auxiliary liquid.
- 14 Tap ✓ **OK**.
  - ➔ The result is displayed.
- 15 Tap ✓ **Finish**.

**See also**

[Settings: application "Density" ▶ Page 92](#)

## 5.4 Adjustments

This section describes how to set up and perform an internal or an external adjustment.

The internal adjustment uses the built-in weights to adjust the balance. Typically, the balance is set to automatically perform an internal adjustment after a certain event.

The external adjustment requires separate weights to adjust the balance. Typically, an external adjustment is only performed when required by the customer's SOP.

≡ **Navigation:** ▼ >  **Applications** >  **Adjustments**

### 5.4.1 Adjustment strategy

This setting defines which adjustment type is performed whenever you start an adjustment.

**Example procedure**

This example shows how to change the adjustment type **Internal** to the adjustment type **External**.

- 1 Open the applications section.
- 2 Tap  **Adjustments**.
- 3 Tap  **External (OFF)**.
  - ➔ The section **Adjustment strategy** opens.
- 4 Select the option **External adjustment**.
- 5 Tap ✓ **Save**.
- 6 Tap  to return to the main weighing screen.

**See also**

[Settings: Adjustment strategy ▶ Page 94](#)

### 5.4.2 Editing an adjustment

This example shows how to edit the adjustment type **Internal**. The procedure to edit the adjustment type **External** is similar.

- 1 Open the applications section.
- 2 Tap  **Adjustments**.
- 3 Tap  **Internal**.
  - ➔ The main weighing screen opens.
- 4 Tap .
- ➔ The section with the settings opens.
- 5 Change the settings according to your needs.
- 6 Tap ✓ **Save**.
  - ➔ The main weighing screen opens.

**See also**

[Adjustment settings ▶ Page 94](#)

### 5.4.3 Performing an internal adjustment

☰ **Navigation:** ▼ > ☰ **Applications** > ⚙ **Adjustments**

■ **Adjustments** is set to **Internal**.

- 1 Option 1: On the main weighing screen, tap ⚙ **Adjust**.  
Option 2: Open the applications section, tap ⚙ **Adjustments**, select the adjustment, and tap ▶ **Start**.
  - ➔ The adjustment is executed.
  - ➔ The adjustment results appear.
- 2 Tap ✓ **Finish**.
  - ➔ The balance is ready.

### 5.4.4 Performing an external adjustment

An external test weight for an external adjustment has to weigh at least 10% of the balance capacity. External test weights under 10% of the balance capacity are not displayed on the balance.

☰ **Navigation:** ▼ > ☰ **Applications** > ⚙ **Adjustments**

This example shows how to define a test weight and how to perform an external adjustment.

■ **Adjustments** is set to **External**.

- 1 On the main weighing screen, tap ⚙ **Adjust**.
- 2 Place the test weight on the weighing pan.
  - ➔ The adjustment is executed.
- 3 When prompted, remove the weight from the weighing pan.
  - ➔ The adjustment results appear.
- 4 Tap ✓ **Finish**.
  - ➔ The balance is ready.

#### See also

🔗 [Settings: External adjustment ▶ Page 95](#)

## 5.5 Tests

Routine tests ensure accurate weighing results according to GWP® or other quality-management systems. The tests should be performed in regular intervals, and the results should be documented in a traceable way.

METTLER TOLEDO can help you to define the routine tests to be performed based on your process requirements. Please contact your local METTLER TOLEDO representative for additional information.

☰ **Navigation:** ▼ > ☰ **Applications** > ⚙

### 5.5.1 Editing a test

This example shows how to edit the sensitivity test. The procedure to edit other routine tests is similar.

- 1 Open the applications section.
- 2 Tap ⚙ **Tests**.
- 3 Tap ⚙ **Sensitivity**.
  - ➔ The main weighing screen opens.
- 4 Tap ⚙.
- ➔ The section with the settings opens.
- 5 Change the settings according to your needs.
- 6 Tap ✓ **OK**.
- 7 Tap ✓ **Save**.
  - ➔ The main weighing screen opens.

### See also

- Settings: Sensitivity test ▶ Page 96
- Settings: Repeatability test ▶ Page 96
- Settings: Eccentricity test ▶ Page 97

## 5.5.2 Performing a test



### NOTICE

#### Incorrect weighing results due to wrong handling of the test weights.

- Only handle test weights with gloves, tweezers, weight forks, or weight handles.

### 5.5.2.1 Sensitivity test

The sensitivity of the balance defines the deviation between the balance reading and the actual load. The sensitivity test allows you to measure the sensitivity using one test point.

≡ **Navigation:** ▼ > **Applications** > **Tests** > **Sensitivity**

This example shows how to perform a sensitivity test with a test point.

- **Test Point** is defined.
- A test weight and an appropriate tool to handle the test weight are available.
  - 1 Open the application **Sensitivity test**.
  - 2 Tap ► **Start**.
    - ➔ The balance is zeroing.
  - 3 Place the test weight on the weighing pan.
  - 4 When prompted, remove the test weight from the weighing pan.
    - ➔ The result is displayed.
  - 5 Tap ✓ **Finish**.

### See also

- Settings: Sensitivity test ▶ Page 96

### 5.5.2.2 Repeatability test

The repeatability test calculates the standard deviation of a series of measurements with a single test weight in order to determine the repeatability of the balance.

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement conditions. During the test, a load is placed and measured at the same location on the weighing pan several times. Afterwards, the difference between the measured weight values is calculated. The spread of the measured results leads to the repeatability.

Repeatability is highly affected by the ambient conditions (drafts, temperature fluctuations and vibrations) and also by the skill of the person performing the weighing. Therefore, the series of measurements must be carried out by the same operator, in the same location, under constant ambient conditions, and without interruption.

≡ **Navigation:** ▼ > **Applications** > **Tests** > **Repeatability**

This example shows how to perform a repeatability test.

- A test weight and an appropriate tool to handle the test weight are available.
  - 1 Open the application **Repeatability test**.
  - 2 If required: Tap the left title section to define the nominal weight of the test weight.
  - 3 Tap ✓ **OK**.

- If required, tap the right title section to define the number of repetitions.

**Note**

Alternatively, tap  to access these settings.

- Tap **✓ Save**.
  - ➔ The main weighing screen opens.
- Tap **▶ Start**.
- Place the test weight on the weighing pan.
- When prompted, remove the test weight.
  - ➔ The balance is zeroing.
- Repeat this procedure as many times as defined.
- When prompted, remove the test weight.
  - ➔ The result is displayed.
- Tap **✓ Finish**.

**See also**

 Settings: Repeatability test ▶ Page 96

### 5.5.2.3 Eccentricity test

The eccentricity test checks if every eccentric load deviation (corner load deviation) is within the user SOP tolerances. The corner load is the deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its distance from the center of the weighing pan (1). If the display remains consistent, even when the same load is placed on different parts of the weighing pan, the balance does not have corner load deviation.

The result corresponds to the highest of the four determined eccentric load deviations (2 to 5).

**Navigation:**  >  **Applications** >  **Tests** >  **Eccentricity**


This example shows how to perform an eccentricity test.

- A test weight and an appropriate tool to handle the test weight are available.
- Open the application **Eccentricity test**.
  - If required: Tap the title section to define the nominal weight of the test weight.

**Note**

Alternatively, tap  to access this setting.

- Tap **▶ Start**.
- When prompted, place the test weight on the appropriate positions of the weighing pan.
- When prompted, remove the test weight.
  - ➔ The result is displayed.
- Tap **✓ Finish**.

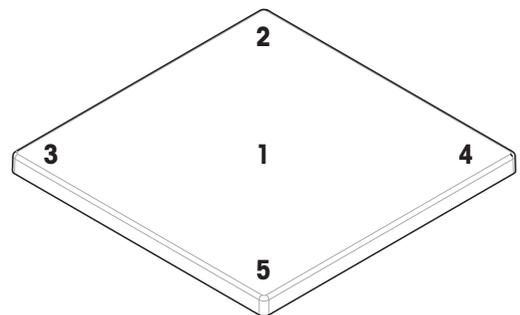

**See also**

 Settings: Eccentricity test ▶ Page 97

## 5.6 Interfaces

### 5.6.1 Ethernet

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 📶 **Interfaces**

This example shows how to configure the balance such that it can communicate with a peripheral device or a service through Ethernet.

- The section **Interfaces** is open.
- 1 Tap the function **Ethernet**.
  - Note**  
This function can be activated or deactivated.
- 2 Tap the parameter **Host name** to change the name.
- 3 Tap ✓ **OK**.
- 4 Tap the parameter **Network configuration**.
- 5 Select the option of your choice.
- 6 Tap ✓ **OK**.
- 7 If you selected the option **Manual**: Change the other parameters if needed, for example, **IP address**.
- 8 Tap ✓ **OK**.
- 9 Tap ✓ **Save**.

#### See also

🔗 [Settings: Interfaces](#) ▶ Page 74

### 5.6.2 Bluetooth

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 📶 **Interfaces**

This example shows how to configure the balance such that it can communicate with a printer through Bluetooth.

#### **Note**

This function is only available if a Bluetooth adapter is connected to the balance.

- A Bluetooth adapter is connected to the balance.
- The section **Interfaces** is open.
- 1 Tap the function **Bluetooth**.
  - Note**  
This function can be activated or deactivated.
- 2 Tap the parameter **Bluetooth identification** to change the name.
- 3 Tap ✓ **OK**.
- 4 Tap ✓ **Save**.

#### See also

🔗 [Settings: Interfaces](#) ▶ Page 74

## 5.7 Devices / Printers

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 🖨️ **Devices / Printers**

#### See also

🔗 [Settings: Devices / Printers](#) ▶ Page 75

🔗 [Accessories](#) ▶ Page 119

## 5.7.1 Printer

Printers serve to document your processes and results. Each weighing application offers the possibility to trigger the printing process manually. The balance can also be configured such that the results are automatically printed.



### NOTICE

#### Damage to the device due to inappropriate use

- Consult the User Manual of the device before using it.

### 5.7.1.1 Installing a printer through RS232

#### Installing and connecting the printer

This example describes how to install an RS232 printer and connect it to the balance.

In contrast to RS232 printers, USB printers are automatically detected by the balance (plug and play).

#### Note

A suitable cable from METTLER TOLEDO must be used to ensure proper function.

#### Navigation: Balance menu > Settings > Devices / Printers

- The RS232 printer is switched on.
- A suitable cable to connect the printer to the balance is available.
- On the balance, the main weighing screen is open.
  - 1 Connect the cable to the RS232 printer.
  - 2 Connect the cable to the RS232 port of the balance.
  - 3 Navigate to the section **Devices / Printers**.
  - 4 Tap **+**.
  - 5 Select the option **RS232**.
  - 6 Tap **→ Next**.
  - 7 Select the option **Printer**.
  - 8 Tap **→ Next**.
  - 9 Select the printer model.
  - 10 Tap **✓**.
  - 11 Configure the printer.
  - 12 Tap **✓**.
    - ➔ The printer appears on the list  **Devices / Printers**.
  - 13 Tap **✓**.
    - ➔ The printer is ready for use.

#### Printing a test page

#### Navigation: Balance menu > Settings > Devices / Printers

- The printer is connected to the balance.
- The main weighing screen is open.
  - 1 Navigate to the section  **Devices / Printers**.
  - 2 Tap the appropriate printer.
  - 3 Tap .
    - ➔ The printer prints a short text.
  - 4 Tap **✓ OK**.

### 5.7.1.2 Installing a printer through Bluetooth

This example describes how to install a printer and connect it to the balance through Bluetooth.



For more information about how to install your Bluetooth adapter, consult the Installation Instructions provided with it.

#### Connecting the printer to the balance

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > 📶 **Interfaces** > 📶 **Bluetooth**

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > 🖨 **Devices / Printers**

- The printer is switched on.
- A Bluetooth RS adapter (to connect to the printer) and a Bluetooth USB adapter (to connect to the balance) are available.
- The switch on the Bluetooth RS adapter is in the position DCE.
- You have identified the MAC address (unique device address) on the Bluetooth RS adapter.
- The main weighing screen is open.

1 Connect the Bluetooth USB adapter (1) to the USB-A port (2) of the balance.

2 Connect the Bluetooth RS adapter (3) to the printer (4).  
➔ The light on the Bluetooth RS adapter starts blinking.

3 Navigate to the section **Bluetooth** and activate the function.

4 Tap ✓ **Save**.

5 Tap 🖨 **Devices / Printers**.

6 Tap +.

7 Select the option **Bluetooth**.

8 Tap → **Next**.

➔ The balance is searching for devices.

9 Select the MAC address of the Bluetooth RS adapter (3).



10 Tap → **Next**.

➔ The balance is pairing the Bluetooth USB adapter (1) with the Bluetooth RS adapter (3) from the printer.

11 Tap → **Next**.

➔ The balance is connecting to the printer.

12 Tap ✓ **Finish**.

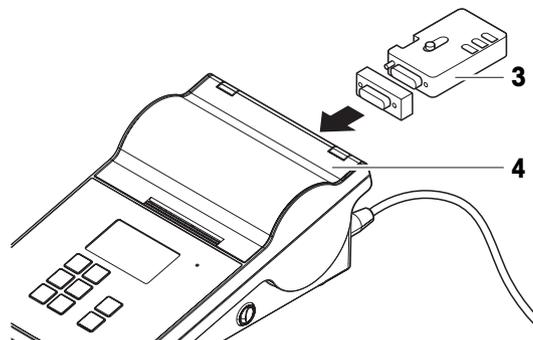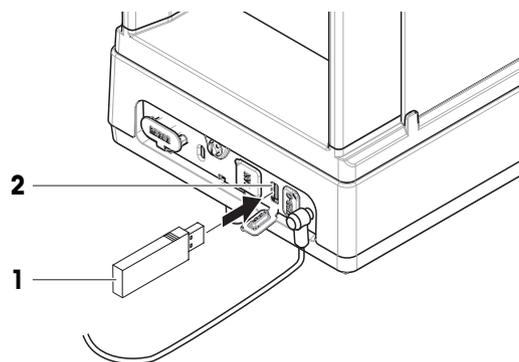

#### Printing a test page

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > 🖨 **Devices / Printers**

- The printer is connected to the balance.
- The main weighing screen is open.

1 Navigate to the section 🖨 **Devices / Printers**.

2 Tap the appropriate printer.

3 Tap ✓.

➔ The printer prints a short text.

4 Tap ✓ **OK**.

#### See also

 Settings: Bluetooth ▶ Page 75

## 5.7.2 Barcode reader

The barcode reader can be used to enter text or numbers in any input field on the display. The format of the field must be compatible with the scanned code.



### NOTICE

#### Damage to the device due to inappropriate use

- Consult the User Manual of the device before using it.

### 5.7.2.1 Scanning a sample ID with a barcode reader

This example shows how to scan a sample ID with a barcode reader in the application **Weighing**.

#### Installing the barcode reader

- A barcode reader is available.
- The main weighing screen is open.
- Connect the USB cable of the barcode reader to the appropriate USB port of the balance.
  - ➔ The balance automatically detects the barcode reader.
  - ➔ The barcode reader appears on the list  **Devices / Printers**.
  - ➔ The barcode reader is ready for use.

#### Scanning a sample ID with the barcode reader

- The barcode reader is configured: **End of line character** is set to "Enter".
- The barcode reader is connected to the balance.
- The application **Weighing** is open.
- 1 Tap  to open the settings.
- 2 Tap  **ID format**.
- 3 Tap **Sample ID**.
- 4 Tap **Default value**.
- 5 Scan the code of the sample ID with the barcode reader.
  - ➔ The scanned sample ID appears in the corresponding field.
- 6 Optional: Tap **Default value** again to manually change the scanned sample ID.
- 7 Tap ✓ **OK**.
- 8 Tap ✓ **Save**.

### 5.7.3 Foot switch

The foot switch can be used to perform certain operations on your balance without having to use the terminal.



### NOTICE

#### Damage to the device due to inappropriate use

- Consult the User Manual of the device before using it.

This example shows how to install and use a foot switch through USB.

### Installing and configuring the foot switch

- A foot switch is available.
- The main weighing screen is open.
- 1 Connect the USB cable of the foot switch to the appropriate USB port of the balance.
  - ➔ The balance automatically detects the foot switch.
  - ➔ The foot switch appears on the list  **Devices / Printers**.
- 2 Tap on the foot switch.
- 3 Tap **Function** and configure how the foot switch is to be used.
- 4 Tap **✓ OK**.
- 5 Tap **✓ Save**.
  - ➔ The foot switch is ready for use.

### 5.7.4 Keyboard

A keyboard can be used to perform certain operations on your balance without having to use the terminal.



#### NOTICE

##### Damage to the device due to inappropriate use

- Consult the User Manual of the device before using it.

This example shows how to install and use a keyboard through USB.

### Installing and configuring the keyboard

- A keyboard with USB cable is available.
- The main weighing screen is open.
- 1 Connect the USB cable of the keyboard to the appropriate USB port of the balance.
  - ➔ The balance automatically detects the keyboard.
  - ➔ The keyboard appears on the list  **Devices / Printers**.
- 2 Tap **✓ OK**.
  - ➔ The keyboard is ready for use.

### 5.7.5 Adding and deleting a device

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** >  **Devices / Printers**

This example shows how to add and delete a printer with a USB interface.

#### Adding a device

- 1 Open the settings section **Devices / Printers**.
- 2 Tap **+**.
- 3 Select the option **USB**.
- 4 Tap **➔ Next**.
- 5 When prompted, connect the device to the balance.
  - ➔ The device is automatically detected.
- 6 Tap **✓ Save**.
  - ➔ The device appears on the list **Devices / Printers**.

#### Deleting a device

- 1 Open the settings section **Devices / Printers**.
- 2 Select the device you want to delete.

- 3 Tap .
- 4 Tap  **OK**.

### 5.7.6 Editing the settings of a device

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > 🖨 **Devices / Printers**

- 1 Open the settings section **Devices / Printers**.
  - ➔ A list of available devices is displayed.
- 2 Adjust the settings if needed.

## 5.8 Services

The balance offers several ways to control the balance remotely or to manage data.

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > ⚙ **Services**

### See also

 [Settings: Services](#) ▶ Page 75

### 5.8.1 MT-SICS service

MT-SICS is a service that allows you to operate the balance by sending commands from a computer. This enables you to integrate your balances into your systems.

The full documentation related to MT-SICS for MX and MR balances is available online.

▶ [www.mt.com/labweighing-software-download](http://www.mt.com/labweighing-software-download)

This example shows how to establish a connection between your balance and a computer through USB. Other connection options work in a similar way. The computer can then be used to control the balance and receive data using the commands of MT-SICS.

#### Configuring the balance

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > ⚙ **Services**

- The section **Services** is open.
- 1 Tap the function **MT-SICS service**.
    -  **Note**  
This function can be activated or deactivated.
  - 2 Tap the setting **Interface**.
  - 3 Select the option **USB**.
  - 4 Tap  **OK**.
  - 5 Tap the setting **Command set**.
  - 6 Select the option **MT-SICS**.
  - 7 Tap  **OK**.
  - 8 Tap  **Save**.

#### Connecting the balance to the computer

When connecting MT-SICS through USB, a USB driver must be installed on your computer. This creates a COM port for communication with the balance.

The USB driver is available online:

▶ [www.mt.com/labweighing-software-download](http://www.mt.com/labweighing-software-download)

- The USB driver is installed on the computer.
  - A terminal program is installed and running on the computer.
  - A suitable cable from METTLER TOLEDO is available.
- 1 Provide the necessary connection settings to the terminal program.
  - 2 Test the connection by sending a command to the balance, for example, `s` to retrieve the stable weight from the balance.
    - ➔ If a string is received by the terminal program with the weight, date, and time, the connection has been successfully established.
    - ➔ If no response is received by the terminal program, check the connection settings.

**See also**

- 🔗 Settings: MT-SICS service ▶ Page 75
- 🔗 Transferring data: MT-SICS service ▶ Page 59

## 5.8.2 EasyDirect Balance

This example shows how to establish a connection between your balance and a computer through USB. The computer can then be used to control the balance and receive data using the software **EasyDirect Balance**.

### Configuring the balance

☰ **Navigation:** ☰ **Balance menu** > ⚙️ **Settings** > ⚙️ **Services**

- The section **Services** is open.
- 1 Tap the function **EasyDirect Balance**.
    - 📘 **Note**  
This function can be activated or deactivated.
  - 2 Tap the setting **Interface**.
  - 3 Select the option **USB**.
  - 4 Tap ✓ **OK**.
  - 5 Tap ✓ **Save**.

### Connecting the balance to the computer

The software **EasyDirect Balance** must be installed on your computer. The software is available online:

▶ [www.mt.com/EasyDirectBalance](http://www.mt.com/EasyDirectBalance)

- A suitable cable from METTLER TOLEDO to connect the balance to the computer is available.
- 1 Install the software **EasyDirect Balance** on your computer.
  - 2 Follow the instructions to establish a connection with the balance.

**See also**

- 🔗 Settings: EasyDirect Balance ▶ Page 76
- 🔗 Transferring data: EasyDirect Balance ▶ Page 60

## 5.8.3 Drop to cursor

This example shows how to configure the balance such that data can be transferred to a computer using the service **Drop to cursor**.

📘 **Note**

The use of special characters is limited when using the service **Drop to cursor**.

## Configuring the balance

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 🔄 **Services**

- The section **Services** is open.
- 1 Tap the service **Drop to cursor**.
  - Note**  
This function can be activated or deactivated.
- 2 Tap the setting **Interface**.
- 3 Select the option **USB**.
- 4 Tap ✓ **OK**.

## Connecting the balance to the computer

- A suitable cable from METTLER TOLEDO is available.
- Connect the balance to the computer.

### See also

- 🔗 Transferring data: Drop to cursor ▶ Page 59
- 🔗 Settings: Drop to cursor ▶ Page 76

## 5.9 Publishing

The balance offers various ways to publish results or transfer data to another device or service. The settings in this section apply to the devices and services that are defined for the balance.

### 5.9.1 Printing data

This setting serves to define a target printer and a print format for printed data.

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 🖨️ **Balance** > 📄 **Publishing**

- A printer is connected to the balance.
- The section **Publishing** is open.
- 1 Tap the function **Printout**.
  - Note**  
This function can be activated or deactivated.
- 2 Tap ✓.

### See also

- 🔗 Settings: Publishing ▶ Page 72

#### 5.9.1.1 Printing results manually through USB

This example shows how to manually print results on a printer that is connected to the balance through USB.

##### **Note**

For printers with an RS232 connection, a suitable RS232 - USB cable from METTLER TOLEDO must be used.

- A printer is connected to the balance through USB.
- A weighing application of your choice is open.
- The section **Report** of the weighing application is configured.
- 1 Place the sample on the weighing pan.
  - ➔ The result is displayed.
- 2 Tap 📄.
  - ➔ The result is printed according to the report configuration.

### See also

[Configuring a report](#) ▶ Page 39

## 5.9.1.2 Printing results automatically through Bluetooth

This example shows how to automatically print results on a printer that is connected to the balance through Bluetooth.

- A printer is connected to the balance through Bluetooth.
- A weighing application of your choice is open, for example, **Weighing**.
- The section **Report** of the weighing application is configured.
  - 1 Navigate to the settings section of the weighing application, for example,  $\Delta\Delta$ .
  - 2 Tap  $\frac{1}{2}$  **Weighing**.
  - 3 Tap **Weight capture mode**.
  - 4 Select the option **Automatic, stable (zero excluded)** or **Automatic, stable (zero included)**.
  - 5 Tap  $\checkmark$ .
    - ➔ The main weighing screen is open.
  - 6 Place a sample on the weighing pan.
    - ➔ The result is printed automatically.

### See also

[Installing a printer through Bluetooth](#) ▶ Page 52

[Configuring a report](#) ▶ Page 39

## 5.9.2 Exporting data to a USB storage device

This setting serves to define a storage location and a file format for exported data.

### **i** Note

Depending on the USB storage device, the export can take up to 15 seconds.

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** >  $\frac{1}{2}$  **Balance** >  $\frac{1}{2}$  **Publishing**

- A USB storage device is connected to the balance.
- The section **Report** of the weighing application is configured.
- The section **Publishing** is open.

- 1 Tap  $\frac{1}{2}$  **Export file**.

### **i** Note

This function can be activated or deactivated.

- 2 Tap the option **Export to** and select a USB storage device.
- 3 Tap the option **File type** and select a format.
- 4 Tap  $\checkmark$ .

### See also

[Settings: Publishing](#) ▶ Page 72

[Configuring a report](#) ▶ Page 39

## 5.9.3 Transferring data to services

This setting serves to define what kind of data is transferred to a target service. Available services are **Drop to cursor**, **MT-SICS service**, and **EasyDirect Balance**.

### See also

[Settings: Publishing](#) ▶ Page 72

### 5.9.3.1 Transferring data: Drop to cursor

The balance offers the option to send weighing results to a computer. This feature can be used, for example, to send results to an Excel sheet or to a text file. With the service **Drop to cursor**, the result is sent to the computer where the cursor is located, as if it were a keyboard input.

#### Configuring the balance

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > ⚖ **Balance** > 📄 **Publishing**

- A computer is connected to the balance.
  - The service **Drop to cursor** is activated and configured.
  - The section **Publishing** is open.
- 1 Tap the function **Transfer data**.
    - 📘 **Note**  
This function can be activated or deactivated.
  - 2 Tap the setting **Transfer to**.
  - 3 Select the option **Drop to cursor**.
  - 4 Tap ✓.
  - 5 In the section **Type of data**, select the type of data you want to transfer.
  - 6 In the section **Field configuration**, define the layout of the transferred data.
  - 7 Tap ✓.

#### Transferring data

In this example, weighing data is transferred to Excel through the service **Drop to cursor**. Which data is transferred is defined here:

≡ **Navigation:** ≡ **Balance menu** > ⚙ **Settings** > 🔄 **Services** > 📄 **Drop to cursor**

- A computer is connected to the balance.
  - The balance is configured as described above.
- 1 On the computer, open Excel and select a target cell.
  - 2 Perform a weighing and tap **Publish**.
    - ➔ The weighing data is added to the target cell in Excel.
  - 3 The next cell is automatically selected for the next weighing data.

#### See also

🔗 [Drop to cursor](#) ▶ Page 56

### 5.9.3.2 Transferring data: MT-SICS service

All MR balances can be integrated into a network. The balance can be configured to communicate with a computer. The service MT-SICS (METTLER TOLEDO Standard Interface Command Set) serves to send commands to operate the balance.

For further information, contact your METTLER TOLEDO representative.

The full documentation related to MT-SICS for MX and MR balances is available online.

▶ [www.mt.com/labweighing-software-download](http://www.mt.com/labweighing-software-download)

## Configuring the balance

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > 📄 **Publishing**

- A computer is connected to the balance.
- The service **MT-SICS** is activated and configured.
- The section **Publishing** is open.
- 1 Tap the function **Transfer data**.
  - Note**  
This function can be activated or deactivated.
- 2 Tap the setting **Transfer to**.
- 3 Select the option **MT-SICS service**.
- 4 Tap ✓.
- 5 Tap the setting **Output mode** and select the option of your choice.
- 6 Tap ✓.

## Transferring data

In this example, weighing data is transferred to the service **MT-SICS**. The data format is defined in **MT-SICS**.

- A computer with **MT-SICS** is connected to the balance.
- The balance is configured as described above.
- Perform a weighing and tap **Publish**.
  - ➔ The weighing data is sent to the **MT-SICS** client.

## See also

🔗 [MT-SICS service](#) ▶ Page 55

### 5.9.3.3 Transferring data: EasyDirect Balance

**EasyDirect Balance** is a software to collect, analyze, store, and export measurement results and balance details from up to ten balances.

## Configuring the balance

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > ⚖️ **Balance** > 📄 **Publishing**

- A computer with the software **EasyDirect Balance** is connected to the balance.
- The service **EasyDirect Balance** is activated and configured.
- The section **Publishing** is open.
- 1 Tap the function **Transfer data**.
  - Note**  
This function can be activated or deactivated.
- 2 Tap the setting **Transfer to**.
- 3 Select the option **EasyDirect Balance**.
- 4 Tap ✓.

## Transferring data

In this example, weighing data is transferred to the software **EasyDirect Balance**. Which data is transferred is defined in the application-specific section **Report**.

- A computer with the software **EasyDirect Balance** is connected to the balance.
- The balance is configured as described above.
- 1 On the computer, open the software **EasyDirect Balance** and select the balance.
- 2 Perform a weighing and tap **Publish**.
  - ➔ The weighing data is sent to the software **EasyDirect Balance**.

### See also

 EasyDirect Balance ▶ Page 56

 Configuring a report ▶ Page 39

## 5.9.4 Publishing options

These settings serve to define how a specific type of result is published. A result type can be, for example, test results.

☰ **Navigation:** ☰ **Balance menu** > ⚙️ **Settings** > ⚙️ **Balance** > 📄 **Publishing**

■ The section **Publishing** is open.

1 Tap **Single results**.

➔ The information is shown that the behavior is defined in the application-specific setting **Weight capture mode**.

2 Tap ✓.

3 Tap **Workflow results**, **Adjustment results**, and/or **Test results**.

4 Select an option.

5 Tap ✓.

### See also

 Settings: Publishing ▶ Page 72

## 5.10 User management



### NOTICE

#### Loss of data due to missing password or user name

Protected menu areas cannot be accessed without user name or password.

– Note user name and password and keep them in a safe place.

### 5.10.1 Activating / deactivating the user management

☰ **Navigation:** ☰ **Balance menu** > ⚙️ **Settings** > ⚙️ **Balance** > ⚙️ **General**

■ The setting **General** is open.

1 Tap the setting **User management**.

2 Select the option **Active** or **Inactive**.

3 Tap ✓ **OK**.

### 5.10.2 Managing users and user groups

☰ **Navigation:** ☰ **Balance menu** > 👤 **User management**

#### 5.10.2.1 Automatic logout

☰ **Navigation:** ☰ **Balance menu** > 👤 **User management** > 👤 **User management – General**

■ The section **User management – General** is open.

1 Tap the setting **Automatic logout**.

##### **Note**

This function can be activated or deactivated.

2 Define a waiting time before automatic logout.

➔ When the balance is not used, the current user is automatically logged out after the defined waiting time.

3 Tap ✓ **Save**.

### See also

 [User management – General ▶ Page 69](#)

## 5.10.2.2 Creating a new user

≡ **Navigation:** ≡ **Balance menu** >  **User management** >  **User management – Users**

- The section **User management – Users** is open.
- 1 Tap **+**.
- 2 Enter a user name.
- 3 Tap **→ Next**.
- 4 Assign a group.
- 5 Tap **→ Next**.
- 6 Optional: Enter the user's first name and last name.
- 7 Select whether the user is currently active or not active.
- 8 Select a language.
- 9 Optional: Set a password.
- 10 Tap **✓ Save**.
  - ➔ The new user appears on the list of users.

### See also

 [User management – Users ▶ Page 69](#)

## 5.10.2.3 Deleting a user

≡ **Navigation:** ≡ **Balance menu** >  **User management** >  **User management – Users**

- The section **User management – Users** is open.
- 1 Tap the user you want to delete.
  - ➔ The user details open.
- 2 Tap .
- 3 Tap **✓ OK**.
  - ➔ The user is removed from the list of users.

## 5.10.2.4 Managing groups

This example shows how to manage permissions for a user group. Whether you are allowed to change these settings depends on your permissions.

≡ **Navigation:** ≡ **Balance menu** >  **User management** >  **User management – Groups**

- The section **User management – Groups** is open.
- 1 Tap a group.
- 2 Tap **Group name** to change the name.
- 3 Tap **Run applications** to select the applications this group is allowed to run.
- 4 Tap **✓ OK**.
- 5 Tap the other settings to activate or deactivate the corresponding permission.
- 6 Tap **✓ Save**.

### See also

 [User management – Groups ▶ Page 69](#)

## 5.11 Password protection

If the function **User management** is activated, each user has an individual password.

- Users can define and change their own password.
- Users with the permission to configure user management can change the password of any user.
- If users forgot their password, they can request a reset.

### 5.11.1 Logging in and logging out

If the function **User management** is activated, users need to log in to use the balance.

#### Logging in

- The login dialog is open.
- 1 Select a user and enter the password.
  - 2 Tap ✓ **OK**.
  - 3 Tap ↪ **Login**.

#### Logging out

- The user is logged in.
- 1 Tap ≡ **Menu**.
  - 2 Tap 👤 **Logout**.

### 5.11.2 Changing a password

≡ **Navigation:** ≡ **Balance menu** > 👤 **User management** > 👤 **User management – Users**

- The user is logged in.
  - The section **User management – Users** is open.
- 1 Tap the appropriate user.
  - 2 Tap 🔑 **Password**.
  - 3 Enter the old password.
  - 4 Tap ✓ **OK**.
  - 5 Enter the new password twice.
  - 6 Tap ✓ **OK**.
  - 7 Tap ✓ **Save**.

### 5.11.3 Resetting a password

If users with the permission to configure the function **User management** have forgotten their password, a password reset can be requested.

- The login dialog is open.
- 1 Tap ⋮ **More**.
  - 2 Tap ↻ **Request reset password**.
  - 3 Enter the user name.
  - 4 Tap ✓ **OK**.
  - 5 Note the service code and tap ✉ **Service request**.
    - ➔ Information about your METTLER TOLEDO service representative appears.
  - 6 Contact your METTLER TOLEDO service representative via phone or email.
    - ➔ You get a temporary password with which you can log in once.
  - 7 Log in with your temporary password and select a new password.

## 5.12 Approved balances

### 5.12.1 Definitions

#### Approved balances

Approved balances are balances that are subject to the local, legal requirements. For approved balances, the net weighing results must comply with a higher level of control. Approved balances are used, for example, for legal metrology, for weight-based trading, or for determination of mass for the application of laws. The term "approved balance" includes legal-for-trade (LFT) balances, certified balances, and registered balances.

The restrictions and special behaviors of these balances are described in the present section as well as in specific balance settings throughout the manual.

To identify approved balances, the characters /M or /A are appended to the model names.

#### Actual scale interval, **d**

The value **d** represents the "actual scale interval". According to OIML R76-1 [T.3.2.2], it represents the difference between two consecutive indicated values. In some countries, the value **d** is defined as the "scale division" or the "scale division interval". In practice, it is often referred to as the "readability".

#### Verification scale interval, **e**

The value **e** represents the "verification scale interval" [OIML R76-1: T.3.2.3]. This value is used for the classification and verification of an instrument. It represents the absolute accuracy of the instrument and is relevant in the context of market surveillance.

The minimum value of the verification scale interval is 1 mg. [OIML R76-1: 3.2]

### 5.12.2 Descriptive markings

The descriptive markings of the instrument are on the type label, according to OIML R76-1 [7.1.4]:

- **Min**: minimum capacity
- **Max**: maximum capacity (referred to as "capacity" in this document)
- **e**: verification scale interval
- **d**: actual scale interval

The type label also contains other metrological characteristics and limits of the instrument.

### 5.12.3 Restrictions on zeroing and taring

#### Zeroing the balance

- When switching on the balance, an initial zero is performed. If the load is more than 20% of the balance capacity during the initial zero, the zeroing is not possible and no weighing value is displayed. [OIML R76-1: T.2.7.2.4 and 4.5.1]
- During operation, the range for which a zero can be performed is  $\pm 2\%$  of the balance capacity. [OIML R76-1: 4.5.1]

#### Taring the balance

- It is not possible to tare the balance if the gross weight is negative. [OIML R76-1: 4.6.4]

### 5.12.4 Application: Weighing

All balances are delivered with an application named **Weighing**. For approved balances:

- The unit of the application **Weighing** can be changed to any available metric unit. Changing the unit requires a restart of the balance.
- When switching on the balance, the application **Weighing** is shown on the weighing screen.
- For the weighing profile used by the application **Weighing**, the setting **Display readability** is **1d** by default. This can be changed, but it will go back to default after a restart of the balance.

## 5.12.5 Representation of weighing results

The representation of weighing results from approved balances follows rules with respect to the weighing units, the weight value, and the indicator of the type of weight. These rules are described in the following paragraphs.

### Unit

A reduced set of units is available for selection.

### Weighing result

If the actual scale interval is smaller than the verification scale interval ( $d < e$ ), the digits that are smaller than  $e$ , are called non-verified digits. For balances showing up to four digits ( $d \geq 0.1$  mg), the non-verified digits are marked. For example, a weight of 100 mg placed on a balance with  $e = 1$  mg and  $d = 0.1$  mg would be printed as 100.[0] mg. [OIML R76-1: 3.4.1, 3.4.2]

- primary weight value on the main weighing screen: the non-verified digits are grayed out
- secondary weight value (**Info weight**) on the main weighing screen: the non-verified digits are grayed out
- **Results list**, detailed view: the non-verified digits are in brackets
- Printout: the non-verified digits are in brackets
- Data export: no special marking

The depiction of the weight values does not affect the accuracy of the weighing results. That is consistent with legal metrology requirements.

### Indicator for weighing result

The type of weighing result, such as **Net weight**, **Tare weight**, or **Gross weight**, is marked according to OIML R76-1 [T.5.2, T.5.3, 4.6.5, 4.6.11, 4.7].

Indicator	Main weighing screen	Printout
<b>Net weight</b>	Net	<b>N</b>
<b>Tare weight</b>	—	<b>T</b>
<b>Preset tare weight</b>	—	<b>PT</b>
<b>Gross weight</b>	—	<b>G</b> <sup>1</sup>
Calculated weight	*	*
Unstable weight	○	<b>D</b>

<sup>1</sup> If only the gross weight is included on the printout, the indicator **G** is omitted.

## 5.12.6 MT-SICS

The following commands are not available for approved balances:

- **C0**
  - It is not possible to change the adjustment type.
- **TI**
  - It is not possible to do an immediate tare. [OIML R76-1: 4.6.8]
- **ZI**
  - It is not possible to do an immediate zero. [OIML R76-1: 4.5.6]

## 5.12.7 Reference

OIML R 76-1 Edition 2006 (E), Non-automatic weighing instruments, Part 1: Metrological and technical requirements – Tests

## 6 Software Description

### 6.1 Balance menu settings

The section **Balance menu** contains general settings and information. To open the section **Balance menu**, tap the symbol  on the main screen.

The section **Balance menu** is divided into the following topics:

-  **Leveling aid**
-  **History**
-  **Information**
-  **User management**
-  **Settings**
-  **Maintenance**

#### 6.1.1 Leveling aid

Exact horizontal positioning and stable installation is essential for repeatable and accurate weighing results. The menu topic **Leveling aid** serves to level the balance.

**Navigation:**  **Balance menu** >  **Leveling aid**

##### **Note**

After leveling the balance, an internal adjustment must be performed.

##### **See also**

 [Leveling the balance](#) ▶ Page 28

#### 6.1.2 History

The balance records the tests and adjustments that are performed in the menu topic **History**.

**Navigation:**  **Balance menu** >  **History**

The menu topic **History** is divided into the following sections.

-  **Adjustments history**
-  **Tests history**
-  **Service history**
-  **Activity log**
-  **Software update history**
-  **Error log**

##### 6.1.2.1 Adjustments history

**Navigation:**  **Balance menu** >  **History** >  **Adjustments**

A maximum of 500 entries can be stored.

Button	Name	Description
	<b>Filter</b>	Tap to filter the list: <ul style="list-style-type: none"><li>• <b>Filter by date</b></li><li>• <b>Filter by user</b></li></ul>
	<b>Publish</b>	Tap to publish or print the displayed entries.

### 6.1.2.2 Tests history

≡ Navigation: ≡ Balance menu > 📄 History > 📄 Tests

A maximum of 500 entries can be stored.

Button	Name	Description
	Filter	Tap to filter the list: <ul style="list-style-type: none"><li>• <b>Filter by date</b></li><li>• <b>Filter by user</b></li></ul>
	Publish	Tap to publish or print the displayed entries.

### 6.1.2.3 Service history

≡ Navigation: ≡ Balance menu > 📄 History > 📄 Service

A maximum of 100 entries can be stored.

Button	Name	Description
	Filter	Tap to filter the list: <ul style="list-style-type: none"><li>• <b>Filter by date</b></li><li>• <b>Filter by user</b></li></ul>
	Publish	Tap to publish or print the displayed entries.

### 6.1.2.4 Activity log

≡ Navigation: ≡ Balance menu > 📄 History > 📄 Activity log

A maximum of 500 entries can be stored.

Button	Name	Description
	Filter	Tap to filter the list: <ul style="list-style-type: none"><li>• <b>Filter by date</b></li><li>• <b>Filter by user</b></li></ul>
	Publish	Tap to publish or print the displayed entries.

### 6.1.2.5 Software update history

≡ Navigation: ≡ Balance menu > 📄 History > 📄 Software update

A maximum of 100 entries can be stored.

Button	Name	Description
	Filter	Tap to filter the list: <ul style="list-style-type: none"><li>• <b>Filter by date</b></li><li>• <b>Filter by user</b></li></ul>

### 6.1.2.6 Error log

≡ Navigation: ≡ Balance menu > 📄 History > 📄 Error log

A maximum of 500 entries can be stored.

Button	Name	Description
	Filter	Tap to filter the list: <ul style="list-style-type: none"><li>• Filter by date</li><li>• Filter by user</li></ul>
	Publish	Tap to publish or print the displayed entries.

### 6.1.3 Information

≡ Navigation: ≡ Balance menu > ⓘ Information

The menu topic **Information** is divided into the following sections:

- 📄 Balance information
- 📧 Service and support information

#### 6.1.3.1 Balance information

≡ Navigation: ≡ Balance menu > ⓘ Information > 📄 Balance information

The section **Balance information** provides information about the following topics:

- Balance identification
- Logged in user (if **User management** activated)
- Software
- Hardware
- Network
- End user license agreement

#### 6.1.3.2 Service and support information

≡ Navigation: ≡ Balance menu > ⓘ Information > 📧 Service and support information

The section **Service and support information** provides information about the following topics:

- Service information
- Service support contact

### 6.1.4 User management

In the menu topic **User management**, rights for users and user groups can be defined. Users can be assigned to user groups.

The menu topic **User management** is only visible if it is activated under the menu topic **Settings**. As a consequence, a login dialog opens at every system start.

A maximum of 10 users can be created. A user is always part of a user group and has the permissions of the corresponding group. Which user has which permissions can be defined or changed by users with the appropriate permission rights.

#### Note

The settings related to screen brightness and sound can be edited by all users and changes are applied to all users. Any user can set a user-specific language for the balance interface without influencing the settings of other users.

### Navigation: Balance menu > User management

The menu topic **User management** is divided into the following sections:

- **User management – General**: settings for all users
- **User management – Users**: settings for individual users
- **User management – Groups**: settings for user groups

#### See also

[User management](#) ▶ Page 61

#### 6.1.4.1 User management – General

##### Navigation: Balance menu > User management > User management – General

Parameter	Description	Values
Automatic logout	Defines whether the user is automatically logged out after a predefined waiting time.	Active   Inactive* Numeric

\* Factory setting

#### 6.1.4.2 User management – Users

##### Navigation: Balance menu > User management > User management – Users

Parameter	Description	Values
User name	Defines a unique identifier for the user. Once the user profile is defined, the value <b>User name</b> cannot be changed anymore.	Text
First name	Defines the first name of the user.	Text
Last name	Defines the last name of the user.	Text
Active	Activates or deactivates the current user.	Active*   Inactive
Assigned group	Assigns the user to user groups.	Defined groups
User language	Defines the language of the user profile.	Available languages
Password	Allows the user to set a password.	Active   Inactive*

\* Factory setting

#### 6.1.4.3 User management – Groups

##### Navigation: Balance menu > User management > User management – Groups

###### Note

This section is only accessible to users with corresponding rights.

Parameter	Description	Values
Group name	Defines the name of the group.	Text (1...22 characters)

###### Activity permissions

Parameter	Description	Values
Run applications	Defines which applications the group is allowed to run.	Active (All)*   Active (number/total number)
Run adjustments	Defines whether the group is allowed to perform adjustments.	Active (All)*   Inactive
Run tests	Defines whether the group is allowed to perform routine tests.	Active (All)*   Inactive
Configure applications	Defines whether the group is allowed to configure applications.	Active   Inactive
Cancel results	Defines whether the group is allowed to cancel results.	Active*   Inactive

Show history	Defines whether the group is allowed to view the menu topic <b>History</b> .	Active   Inactive
--------------	--	-------------------

\* Factory setting

### General configuration permissions

Parameter	Description	Values
Quality management	Defines whether the group is allowed to configure the balance settings <b>Weighing / Quality</b> .	Active   Inactive
User management	Defines whether the group is allowed to configure settings of the menu topic <b>User management</b> .	Active   Inactive
General	Defines whether the group is allowed to configure the balance settings <b>General</b> .	Active   Inactive

## 6.1.5 Settings

This section describes the settings of the balance that can be changed to suit specific requirements. The balance settings apply to the entire weighing system and to all users.

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings**

The menu topic **Settings** is divided into the following sections:

- 🏠 **Balance**
- 🖨️ **Interfaces**
- 🖨️ **Devices / Printers**
- ⚙️ **Services**

### 6.1.5.1 Settings: Balance

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 🏠 **Balance**

The section **Balance** is divided into the following subsections:

- ⚖️ **Weighing / Quality**
- 🖨️ **Publishing**
- 🕒 **Date / Time / Language**
- 🔊 **Screen / Sound**
- ⚙️ **General**

#### 6.1.5.1.1 Settings: Weighing / Quality

≡ **Navigation:** ≡ **Balance menu** > ⚙️ **Settings** > 🏠 **Balance** > ⚖️ **Weighing / Quality**

Parameter	Description	Values
Leveling warning	Defines the action when the balance is out of level. For approved balances, this setting is set to <b>Forced leveling</b> and cannot be edited.	Active*   Inactive Optional leveling*   Forced leveling
Weighing profiles	A weighing profile stores the balance settings needed for a certain weighing application. It is possible to create separate weighing profiles for different weighing applications. Detailed settings are described in the table <b>Weighing profiles</b> below.	Weighing profile 2, Weighing profile 3: Active   Inactive
Service reminder	Defines whether the user is reminded about the upcoming due date of the service.	Active*   Inactive

\* Factory setting

## Weighing profiles

Settings related to weighing performance and data from balance calibration can be stored in a weighing profile.

Parameter	Description	Values
Name	Defines the name of the profile.	Text (1...22 characters)
Environment	<p>Defines the environmental conditions of the balance.</p> <p><b>Very stable:</b> For an environment that is free from any drafts and vibrations.</p> <p><b>Stable:</b> For an environment that is practically free from drafts and vibrations.</p> <p><b>Standard:</b> For an average working environment subject to moderate variations in the ambient conditions.</p> <p><b>Very unstable:</b> For an environment where the conditions are from time to time changing.</p>	Very stable   Stable   Standard*   Unstable   Very unstable
Weighing mode	<p>Defines the filter settings of the balance.</p> <p><b>Universal:</b> For all standard weighing applications.</p> <p><b>Sensor mode:</b> Depending on the setting of the ambient conditions, this setting delivers a filtered weighing signal of varying strength. The filter has a linear characteristic in relation to time (not adaptive) and is suitable for continuous measured value processing.</p>	Universal*   Sensor mode
Value release	<p>Defines the speed at which the balance regards the measured value as stable and available for capture.</p> <p><b>Very fast:</b> Recommended if you require fast results and repeatability is not very important.</p> <p><b>Very reliable:</b> Provides very good repeatability of measurement results, but increases stabilization time.</p>	Very fast   Fast   Fast and reliable*   Reliable   Very reliable
Display readability	<p>Determines the readability d of the balance display.</p> <p>1d: maximum resolution            2d: 2 times smaller resolution            5d: 5 times smaller resolution            10d: 10 times smaller resolution            20d: 20 times smaller resolution            50d: 50 times smaller resolution            100d: 100 times smaller resolution            200d: 200 times smaller resolution            500d: 500 times smaller resolution            1000d: 1000 times smaller resolution</p> <p>For approved balances, the values available for this setting depend on the balance model.</p>	1d*   2d   5d   10d   20d   50d   100d   200d   500d   1000d
Zero drift compensation	<p>Performs ongoing corrections of deviations from zero. Such drifts can occur, for example, as a result of small amounts of dirt on the weighing pan.</p> <p>For approved balances, the values available for this setting depend on the balance model.</p>	Active*   Inactive
Smallest net weight	Defines the smallest net weight [g].	Active   Inactive* Numeric

\* Factory setting

### 6.1.5.1.2 Settings: Publishing

Navigation: ≡ Balance menu > ⚙ Settings > ⚖ Balance > 📄 Publishing

Parameter	Description	Values
Printout	<b>Print to:</b> Defines on which printer the results are printed. <b>Printout type:</b> Defines how the results are printed.	Active*   Inactive
Export file	<b>Export to:</b> Defines where the results are exported to. <b>File type:</b> Defines the type of the export file (csv, txt).	Active   Inactive*
Transfer data	<b>Transfer to:</b> Defines where the results are transferred to when being published. Detailed settings are described in the tables <b>Type of data</b> and <b>Field configuration</b> below.	Active   Inactive* Drop to cursor   MT-SICS service   EasyDirect Balance

\* Factory setting

#### Publishing options

These settings apply to all available publishing options.

Parameter	Description	Values
Single results	Single results are published as defined in the setting <b>Weight capture mode</b> .	Application specific
Workflow results	Defines whether the workflow results are published immediately after the result is calculated.	Automatic*   Manual
Adjustment results	Defines whether the adjustment results are published immediately after the result is calculated.	Automatic   Manual*
Test results	Defines whether the test results are published immediately after the result is calculated.	Automatic   Manual*
Approval brackets	Indicates uncertified digits. Relevant for approved balances only.	Active   Inactive* <ul style="list-style-type: none"> <li>• [ ] : first decimal place</li> <li>• [ ] : first decimal place for dual range balances</li> </ul>

\* Factory setting

#### Type of data

Parameter	Description	Values
Sample ID, Description ID 1, Description ID 2, Description ID 3, Date, Time	Defines whether the corresponding field is included in the output.	Active   Inactive*

\* Factory setting

#### Field configuration

Parameter	Description	Values
Weight status	Defines whether the weight status is included in the output.	Active   Inactive*
Sign	Defines whether the weighing results are published with a plus sign or a minus sign to indicate positive or negative values.	Always   Only negative values*
Decimal delimiter	Defines the character used to separate decimal values.	, (comma)   . (full stop)*
Net indicator	Defines whether the net weights are specially marked in the output.	Active   Inactive*

Unit	Defines whether the weighing results are published with a unit.	Active*   Inactive
Field delimiter	Defines the character used to separate data fields.	None   TAB*   , (comma)   ; (semicolon)   SPACE
End of line character	Defines the character used at the end of a line.	TAB   Enter*   None

\* Factory setting

### See also

 Publishing ▶ Page 57

## 6.1.5.1.3 Settings: Date / Time / Language

≡ Navigation: ≡ Balance menu > ⚙ Settings > ⚖ Balance > 🕒 Date / Time / Language

Parameter	Description	Values
Date	Defines the current date.	Date
Time	Defines the current time.	Time
Language	Defines the language of the interface navigation.	English*   Deutsch   Français   Español   Italiano   Polski   Český   Magyar   Nederlands   Português   Türkçe   中文   日本語   한국어
Show date / time	Shows the current date and time on the screen, in the defined format.	Active*   Inactive
Time zone	Selects a time zone. When the time zone is set, the balance changes automatically between summer and winter time. When this parameter is activated, the setting <b>Time synchronization</b> becomes available. This enables synchronization with an NTP server in the network.	Active   Inactive*
Date format	Defines the date format.	DD.MM.YYYY*   MM/DD/YYYY   YYYY-MM-DD   YYYY/MM/DD
Time format	Defines the time format.	24:MM*   12:MM   24.MM   12.MM

\* Factory setting

## 6.1.5.1.4 Settings: Screen / Sound

≡ Navigation: ≡ Balance menu > ⚙ Settings > ⚖ Balance > 📺 Screen / Sound

Parameter	Description	Values
Screen brightness	Defines the brightness of the display.	10% ... 100%
Sound volume	Defines the volume of the sound.	Inactive   Low   Medium*   High
Sound on key press	Defines whether a sound is audible when a key is pressed.	Active*   Inactive
Sound on feedback	Defines whether a sound is audible when an information appears on the display.	Active*   Inactive

Sound on stability	Defines whether a sound is audible when the weight value becomes stable.	Active*   Inactive
--------------------	--	--------------------

\* Factory setting

### 6.1.5.1.5 Settings: General

Navigation: Balance menu > Settings > Balance > General

Parameter	Description	Values
Balance ID	Defines the ID of the balance. This name can be used to communicate with the balance over a network. No space or special characters are allowed.	Text (1...24 characters)
Standby	Defines the time before the balance goes into standby mode when it is not in use.	Active*   Inactive Numeric
Power-saving mode	Defines the working hours and working days. Outside of the defined times, the balance goes into power-saving mode. The setting <b>Start work</b> defines when the balance is ready for use.	Active   Inactive*
Communication	Defines whether the balance interfaces are open or blocked for communication with connected devices.	Active*   Blocked
User management	Activates or deactivates the menu topic <b>User management</b> .	Active*   Inactive

\* Factory setting

### 6.1.5.2 Settings: Interfaces

Navigation: Balance menu > Settings > Interfaces

The section **Interfaces** is divided into the following subsections:

- Ethernet
- Bluetooth

Parameter	Description	Values
Ethernet	With the option <b>Ethernet</b> , the balance can communicate with peripheral devices, such as a printer.	Active   Inactive*
Bluetooth	With the option <b>Bluetooth</b> , the balance can communicate with peripheral devices, such as a printer.	Active   Inactive*

\* Factory setting

#### See also

Interfaces ▶ Page 50

### 6.1.5.2.1 Settings: Ethernet

The interface **Ethernet** allows to connect the balance to a network and perform the following actions:

- store weighing results as XML files on a share folder
- communicate remotely with the balance using the MT-SICS communication protocol or LabX

Navigation: Balance menu > Settings > Interfaces > Ethernet

Parameter	Description	Values
Host name	Defines the host name of the balance.	Text (1...24 characters)
MAC address	Information on the MAC address that is used to uniquely identify the balance in the network.	not editable

Network configuration	<b>DHCP:</b> The settings of the Ethernet connection will be automatically set. <b>Manual:</b> The settings of the Ethernet connection must be set manually by the user. If this option is selected, the following parameters are editable.	DHCP*   Manual
IP address	Defines the IP address of the balance.	000.000.000.000... 255.255.255.255
Subnet mask	Defines the subnet mask that is used by the TCP/IP protocol to determine whether a host is on the local subnet or on a remote network.	000.000.000.000... 255.255.255.255
DNS server	Defines the address of the DNS (domain name system) server.	000.000.000.000... 255.255.255.255
Standard gateway	Defines the address of the standard gateway that links the subnet of the host to other networks.	000.000.000.000... 255.255.255.255

\* Factory setting

### 6.1.5.2.2 Settings: Bluetooth

Navigation: Balance menu > Settings > Interfaces > Bluetooth

Parameter	Description	Values
Bluetooth identification	Serves to identify the balance when the option <b>Bluetooth</b> is used.	Text (1...24 characters)

### 6.1.5.3 Settings: Devices / Printers

Navigation: Balance menu > Settings > Devices / Printers

Parameter	Description	Values
Physical connection	Defines the type of physical connection between the balance and a peripheral device.	USB*   RS232   USB-RS232 converter   Network

\* Factory setting

### 6.1.5.4 Settings: Services

Several services are available to communicate with the balance. Note that only one service can be enabled at any given time.

Navigation: Balance menu > Settings > Services

The section **Services** is divided into the following subsections:

-  **MT-SICS service**
-  **EasyDirect Balance**
-  **Drop to cursor**

See also

[Services](#) ▶ Page 55

#### 6.1.5.4.1 Settings: MT-SICS service

Navigation: Balance menu > Settings > Services >  **MT-SICS service**

Parameter	Description	Values
Interface	If the option <b>MT-SICS service</b> is activated, a corresponding port is opened.	USB   RS232   USB-RS232 converter*   Network

Command set	Available set of commands to communicate with the balance.	MT-SICS*   Sartorius commands 22   Sartorius commands 16
Baudrate	Defines the speed of data transmission.	600 bps   1200 bps   2400 bps   4800 bps   9600 bps *   19200 bps   38400 bps   57600 bps   115200 bps
Bits/Parity	Number of data bits / Checksum for error detection during data transmission	8/No*   7/No   7/Even   7/Odd
Data flow	Also known as "handshake". Defines the synchronization for data transmission.	Xon/Xoff*   RTS/CTS   None
Stop bit	Marks the end of data transmission.	1 bit*   2 bit
Line end	Defines the character at the end of a line.	<CR><LF>*   <CR>   <LF>   <TAB>

\* Factory setting

#### See also

[🔗](#) MT-SICS service ▶ Page 55

### 6.1.5.4.2 Settings: EasyDirect Balance

☰ **Navigation:** ☰ **Balance menu** > ⚙️ **Settings** > ⚙️ **Services** > 🖨️ **EasyDirect Balance**

Parameter	Description	Values
Interface	The option <b>EasyDirect Balance</b> can only communicate with the balance through USB.	USB*   RS232

\* Factory setting

#### See also

[🔗](#) EasyDirect Balance ▶ Page 56

### 6.1.5.4.3 Settings: Drop to cursor

☰ **Navigation:** ☰ **Balance menu** > ⚙️ **Settings** > ⚙️ **Services** > 🖨️ **Drop to cursor**

Parameter	Description	Values
Interface	The option <b>Drop to cursor</b> can only be used through USB.	USB*

\* Factory setting

#### See also

[🔗](#) Drop to cursor ▶ Page 56

## 6.1.6 Maintenance

☰ **Navigation:** ☰ **Balance menu** > 🛠️ **Maintenance**

#### **Note**

This section is only accessible to users with corresponding rights.

The menu topic **Maintenance** is divided into the following sections:

- 🔄 **Import / Export**
- 📄 **Software update**
- ↺ **Reset**
- 📁 **Save support file**

-  **Level center adjustment**
-  **Service tool connection**

**See also**


-  [Exporting data to a USB storage device](#) ▶ Page 58
-  [Updating the software](#) ▶ Page 104
-  [Resetting the balance](#) ▶ Page 105
-  [Saving a support file](#) ▶ Page 110

## 6.2 Weighing applications settings

### 6.2.1 Settings: application "Weighing"

This section describes the settings of the application **Weighing**.

≡ **Navigation:** ▼ >  >  **Weighing** > 

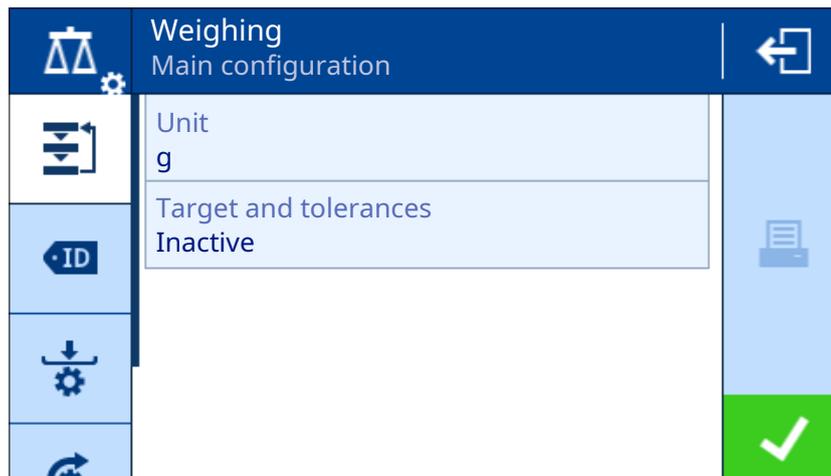

The settings for this weighing application are grouped as follows:

-  **Main configuration**
-  **ID format**
-  **Weighing configuration**
-  **Automation**
-  **Report configuration**

**See also**

-  [Application "Weighing"](#) ▶ Page 40

#### 6.2.1.1 Main configuration

Parameter	Description	Values
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.
Target and tolerances	The target weight can be added manually or by weighing. The definition of tolerances is optional. Depending on the settings, the target weight and the tolerance limits appear on the main weighing screen. The section SmartTrac indicates whether the current weighing result is within the tolerance limits.	Active   Inactive* Numeric Tolerances: %   g

\* Factory setting

## 6.2.1.2 ID format

### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

## 6.2.1.3 Weighing configuration

Parameter	Description	Values
Info weight	A secondary weight is displayed on the main weighing screen.	Active   Inactive* The available units depend on the balance model.
Weighing profile	Defines the weighing profile.	General*   10d
Weight capture mode	Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation. <b>Stable:</b> The balance waits for a stable weight. <b>Immediate:</b> The balance does not wait for a stable weight. <b>Automatic, stable (zero excluded):</b> The results are published as soon as the weight is stable. Values of 0 g are not published. <b>Automatic, stable (zero included):</b> The results are published as soon as the weight is stable. Values of 0 g are also published.	Stable*   Immediate   Automatic, stable (zero excluded)   Automatic, stable (zero included)

\* Factory setting

### Series / Statistics

Parameter	Description	Values
Measurement series	A measurement series can be performed.	Active   Inactive*
Statistical calculations	Statistical information is provided. This setting is only available if the parameter <b>Measurement series</b> is activated.	Active   Inactive*

Acceptance range	Defines the acceptance range for the statistical calculations. This setting is only available if the parameter Statistical calculations is activated.	Active   Inactive* Numeric (%)
------------------	--	-----------------------------------

\* Factory setting

#### See also

[Weighing profiles](#) ▶ Page 35

### 6.2.1.4 Automation

Parameter	Description	Values
Automatic zero	The balance is automatically zeroed when the weight falls below a predefined threshold. This setting is not available for approved balances.	Active   Inactive* Numeric The available units depend on the balance model.
Automatic tare	The balance automatically stores the first stable weight as the tare weight.	Active   Inactive*
Recall weight	Displays the last weighing result.	Active   Inactive* Automatic   Manual*

\* Factory setting

### 6.2.1.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state   Tolerance state
Task information	Defines which information about the task is published.	Application settings
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Info weight   Date/time

## 6.2.2 Settings: application "Counting"

This section describes the settings of the application **Counting**.

☰ **Navigation:** ▼ > > **Counting** >

The settings for this weighing application are grouped as follows:

- **Main configuration**
- **ID format**
- **Weighing configuration**
- **Automation**
- **Report configuration**

#### See also

[Application "Counting"](#) ▶ Page 40

### 6.2.2.1 Main configuration

Parameter	Description	Values
Reference PCS	Defines the number of items used to determine the average weight per item.	Numeric
Reference average weight	Defines the average weight for one piece. The average weight of one piece serves as the basis for piece counting. During task execution, the balance calculates the actual number of pieces on the weighing pan based on the measured weight and the average weight of one piece.	Numeric
Target and tolerances	The target weight can be added manually or by weighing. The definition of tolerances is optional.  Depending on the settings, the target weight and the tolerance limits appear on the main weighing screen. The section SmartTrac indicates whether the current weighing result is within the tolerance limits.	Active   Inactive* Numeric Tolerances: PCS   %

\* Factory setting

### 6.2.2.2 ID format

#### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

#### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

### 6.2.2.3 Weighing configuration

Parameter	Description	Values
Info weight	A secondary weight is displayed on the main weighing screen.	Active   Inactive* The available units depend on the balance model.
Weighing profile	Defines the weighing profile.	General*   10d

Weight capture mode	<p>Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation.</p> <p><b>Stable:</b> The balance waits for a stable weight.</p> <p><b>Immediate:</b> The balance does not wait for a stable weight.</p> <p><b>Automatic, stable (zero excluded):</b> The results are published as soon as the weight is stable. Values of 0 g are not published.</p> <p><b>Automatic, stable (zero included):</b> The results are published as soon as the weight is stable. Values of 0 g are also published.</p>	Stable*   Immediate   Automatic, stable (zero excluded)   Automatic, stable (zero included)
---------------------	---	---

\* Factory setting

### Series / Statistics

Parameter	Description	Values
Measurement series	A measurement series can be performed.	Active   Inactive*
Statistical calculations	<p>Statistical information is provided.</p> <p>This setting is only available if the parameter <b>Measurement series</b> is activated.</p>	Active   Inactive*
Acceptance range	<p>Defines the acceptance range for the statistical calculations.</p> <p>This setting is only available if the parameter Statistical calculations is activated.</p>	Active   Inactive* Numeric (%)

\* Factory setting

### See also

[🔗 Weighing profiles](#) ▶ Page 35

#### 6.2.2.4 Automation

Parameter	Description	Values
Automatic zero	<p>The balance is automatically zeroed when the weight falls below a predefined threshold.</p> <p>This setting is not available for approved balances.</p>	Active   Inactive* Numeric The available units depend on the balance model.
Automatic tare	The balance automatically stores the first stable weight as the tare weight.	Active   Inactive*
Recall weight	Displays the last weighing result.	Active   Inactive* Automatic   Manual*

\* Factory setting

#### 6.2.2.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state   Tolerance state

Task information	Defines which information about the task is published.	Application settings
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Info weight   Date/time

### 6.2.3 Settings: application "Check weighing"

This section describes the settings of the application **Check weighing**.

☰ **Navigation:** ▼ >  >  **Check weighing** > 

The settings for this weighing application are grouped as follows:

-  **Main configuration**
-  **ID format**
-  **Weighing configuration**
-  **Automation**
-  **Report configuration**

#### See also

 Application "Check weighing" ▶ Page 41

#### 6.2.3.1 Main configuration

Parameter	Description	Values
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.
Target weight ± Tolerances	The target weight can be added manually or by weighing. The definition of tolerances is optional. Depending on the settings, the target weight and the tolerance limits appear on the main weighing screen. The section SmartTrac indicates whether the current weighing result is within the tolerance limits.	Numeric Tolerances: Active*   Inactive %   g
Check threshold	Defines the target threshold. Values below the defined threshold are not checked.	Active*   Inactive Numeric (%)

\* Factory setting

#### 6.2.3.2 ID format

##### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

##### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series

Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

### 6.2.3.3 Weighing configuration

Parameter	Description	Values
Info weight	A secondary weight is displayed on the main weighing screen.	Active   Inactive* The available units depend on the balance model.
Weighing profile	Defines the weighing profile.	General*   10d
Weight capture mode	Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation. <b>Stable:</b> The balance waits for a stable weight. <b>Immediate:</b> The balance does not wait for a stable weight. <b>Automatic, stable (zero excluded):</b> The results are published as soon as the weight is stable. Values of 0 g are not published. <b>Automatic, stable (zero included):</b> The results are published as soon as the weight is stable. Values of 0 g are also published.	Stable*   Immediate   Automatic, stable (zero excluded)   Automatic, stable (zero included)

\* Factory setting

### Series / Statistics

Parameter	Description	Values
Measurement series	A measurement series can be performed.	Active   Inactive*
Statistical calculations	Statistical information is provided. This setting is only available if the parameter <b>Measurement series</b> is activated.	Active   Inactive*
Acceptance range	Defines the acceptance range for the statistical calculations. This setting is only available if the parameter Statistical calculations is activated.	Active   Inactive* Numeric (%)

\* Factory setting

### See also

[Weighing profiles](#) ▶ Page 35

### 6.2.3.4 Automation

Parameter	Description	Values
Automatic zero	The balance is automatically zeroed when the weight falls below a predefined threshold. This setting is not available for approved balances.	Active   Inactive* Numeric The available units depend on the balance model.
Automatic tare	The balance automatically stores the first stable weight as the tare weight.	Active   Inactive*

Recall weight	Displays the last weighing result.	Active   Inactive* Automatic   Manual*
---------------	------------------------------------	---

\* Factory setting

### 6.2.3.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state   Tolerance state
Task information	Defines which information about the task is published.	Application settings
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Info weight   Date/time

### 6.2.4 Settings: application "Dynamic weighing"

This section describes the settings of the application **Dynamic weighing**.

☰ **Navigation:** ▼ >  >  **Dynamic weighing** > 

The settings for this weighing application are grouped as follows:

-  **Main configuration**
-  **ID format**
-  **Weighing configuration**
-  **Automation**
-  **Report configuration**

#### See also

 Application "Dynamic weighing" ▶ Page 42

#### 6.2.4.1 Main configuration

Parameter	Description	Values
Measurement duration	Defines the measuring duration in seconds.	Numeric
Start mode	Defines how the measurement is started.	Manual   Automatic - After 3 seconds*
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.

\* Factory setting

## 6.2.4.2 ID format

### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

## 6.2.4.3 Weighing configuration

Parameter	Description	Values
Info weight	A secondary weight is displayed on the main weighing screen.	Active   Inactive* The available units depend on the balance model.
Weighing profile	Defines the weighing profile.	General*   10d

\* Factory setting

### Series / Statistics

Parameter	Description	Values
Measurement series	A measurement series can be performed.	Active   Inactive*
Statistical calculations	Statistical information is provided. This setting is only available if the parameter <b>Measurement series</b> is activated.	Active   Inactive*
Acceptance range	Defines the acceptance range for the statistical calculations. This setting is only available if the parameter Statistical calculations is activated.	Active   Inactive* Numeric (%)

\* Factory setting

## 6.2.4.4 Automation

Parameter	Description	Values
Sample tare	After the result has been calculated, the balance is automatically tared when the sample is removed from the weighing pan.	Active   Inactive

Automatic zero	The balance is automatically zeroed when the weight falls below a predefined threshold. This setting is not available for approved balances.	Active   Inactive* Numeric The available units depend on the balance model.
Automatic tare	The balance automatically stores the first stable weight as the tare weight.	Active   Inactive*

\* Factory setting

### 6.2.4.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state
Task information	Defines which information about the task is published.	Application settings
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Info weight   Date/time

### 6.2.5 Settings: application "Formulation"

This section describes the settings of the application **Formulation**.

≡ **Navigation:** ▼ >  >  **Formulation** > 

The settings for this weighing application are grouped as follows:

-  **Main configuration**
-  **ID format**
-  **Weighing configuration**
-  **Automation**
-  **Report configuration**

**See also**

 [Application "Formulation" ▶ Page 43](#)

#### 6.2.5.1 Main configuration

Parameter	Description	Values
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.

### 6.2.5.2 ID format

#### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

#### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

### 6.2.5.3 Weighing configuration

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Weight capture mode	Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation. <b>Stable:</b> The balance waits for a stable weight. <b>Immediate:</b> The balance does not wait for a stable weight.	Stable*   Immediate

\* Factory setting

### 6.2.5.4 Automation

Parameter	Description	Values
Automatic zero	The balance is automatically zeroed when the weight falls below a predefined threshold. This setting is not available for approved balances.	Active   Inactive* Numeric The available units depend on the balance model.

\* Factory setting

### 6.2.5.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines

Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Date/time

## 6.2.6 Settings: application "Totaling"

This section describes the settings of the application **Totaling**.

☰ **Navigation:** ▼ >  > **Totaling** > 

The settings for this weighing application are grouped as follows:

- ☰ **Main configuration**
- 🗉 **ID format**
- ⚙️ **Weighing configuration**
- ⌚ **Automation**
- 📄 **Report configuration**

### See also

[Application "Totaling"](#) ▶ Page 44

### 6.2.6.1 Main configuration

Parameter	Description	Values
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.

### 6.2.6.2 ID format

#### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

#### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)

Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

### 6.2.6.3 Weighing configuration

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Weight capture mode	Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation. <b>Stable:</b> The balance waits for a stable weight. <b>Immediate:</b> The balance does not wait for a stable weight. <b>Automatic, stable (zero excluded):</b> The results are published as soon as the weight is stable. Values of 0 g are not published. <b>Automatic, stable (zero included):</b> The results are published as soon as the weight is stable. Values of 0 g are also published.	Stable*   Immediate   Automatic, stable (zero excluded)   Automatic, stable (zero included)

\* Factory setting

### 6.2.6.4 Automation

Parameter	Description	Values
Automatic zero	The balance is automatically zeroed when the weight falls below a predefined threshold. This setting is not available for approved balances.	Active   Inactive* Numeric The available units depend on the balance model.
Automatic tare	The balance automatically stores the first stable weight as the tare weight.	Active   Inactive*

\* Factory setting

### 6.2.6.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Date/time

### 6.2.7 Settings: application "Back weighing"

This section describes the settings of the application **Back weighing**.

Navigation: > > **Back weighing** >

The settings for this weighing application are grouped as follows:

- **Main configuration**
- **ID format**
- **Weighing configuration**
- **Automation**
- **Report configuration**

#### See also

Application "Back weighing" ▶ Page 44

### 6.2.7.1 Main configuration

Parameter	Description	Values
Tare container	Defines whether a tare container is used.	Active*   Inactive
Difference unit	Selects the result view for the calculated difference. <b>Percentage (%)</b> : Reports the difference between back-weighing and initial weighing as a percentage of the initial weight. <b>Absolute percentage (% Abs.)</b> : Reports back-weighing as a percentage of the initial weight. <b>ATRO moisture content (%AM)</b> : Reports the moisture content of the sample as a percentage of the dry weight. <b>ATRO dry content (%AD)</b> : Reports the wet weight of the sample as a percentage of the dry weight.	Weight*   Percentage (%)   Absolute percentage (% Abs.)   ATRO moisture content (%AM)   ATRO dry content (%AD)
Difference value	Displays the calculated difference in work area and result view. <b>Unsigned (absolute value)</b> : Displays the absolute value. <b>Signed</b> : Displays the value by means of algebraic sign.	Unsigned (absolute value)*   Signed

\* Factory setting

#### Initial values for weighing

Parameter	Description	Values
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.

\* Factory setting

### 6.2.7.2 ID format

#### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

## Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

### 6.2.7.3 Weighing configuration

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Weight capture mode	<p>Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation.</p> <p><b>Stable:</b> The balance waits for a stable weight.</p> <p><b>Immediate:</b> The balance does not wait for a stable weight.</p> <p><b>Automatic, stable (zero excluded):</b> The results are published as soon as the weight is stable. Values of 0 g are not published.</p> <p><b>Automatic, stable (zero included):</b> The results are published as soon as the weight is stable. Values of 0 g are also published.</p>	Stable   Immediate   Automatic, stable (zero excluded)*   Automatic, stable (zero included)

\* Factory setting

### Series / Statistics

Parameter	Description	Values
Measurement series	A measurement series can be performed.	Active   Inactive*
Statistical calculations	<p>Statistical information is provided.</p> <p>This setting is only available if the parameter <b>Measurement series</b> is activated.</p>	Active   Inactive*
Acceptance range	<p>Defines the acceptance range for the statistical calculations.</p> <p>This setting is only available if the parameter Statistical calculations is activated.</p>	Active   Inactive* Numeric (%)

\* Factory setting

### 6.2.7.4 Automation

Parameter	Description	Values
Automatic zero	<p>The balance is automatically zeroed when the weight falls below a predefined threshold.</p> <p>This setting is not available for approved balances.</p>	Active   Inactive* Numeric The available units depend on the balance model.

\* Factory setting

## 6.2.7.5 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state
Task information	Defines which information about the task is published.	Application settings   Measurement details
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Date/time

## 6.2.8 Settings: application "Density"

This section describes the settings of the application **Density**.

☰ **Navigation:** ▼ >  > **Density** > .

The settings for this weighing application are grouped as follows:

-  **Main configuration**
-  **ID format**
-  **Weighing configuration**
-  **Report configuration**

### See also

[Application "Density" ▶ Page 45](#)

### 6.2.8.1 Main configuration

Parameter	Description	Values
Determination type	Defines the type of density measurement.	Solid*
Density result	Defines the number of decimal places of the result value.	1 decimal place   2 decimal places   3 decimal places   4 decimal places

\* Factory setting

### Initial values for weighing

Parameter	Description	Values
Unit	Defines the unit of the weighing result.	The available units depend on the balance model.
Auxiliary liquid	Defines the type of auxiliary liquid used.	Distilled water*   Custom
Temperature	Defines the temperature of the auxiliary liquid.	Numeric (°C)
Auxiliary liquid density	Defines the density of the auxiliary liquid. For distilled water, the value is predefined.	Numeric (g/cm <sup>3</sup> )

\* Factory setting

## 6.2.8.2 ID format

### Sample ID

Parameter	Description	Values
Sample ID	Allows to define a sample identification.	Active   Inactive* Text (1...194 characters)
Default value	Defines a default value for the sample description.	Text (1...18 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	not editable
Input prompt	Defines whether you are prompted to enter a value.	not editable

\* Factory setting

### Description

Parameter	Description	Values
Description	Allows to define a sample description.	Active   Inactive*
Type	Defines the sample type.	Sample*   Series
Label	Describes the sample.	Text (1...24 characters)
Default value	Defines a default value for the sample description.	Text (1...24 characters)
Automatic value	Defines whether an automatic value is generated for the sample description.	Active   Inactive*
Input prompt	Defines whether you are prompted to enter a value.	Active*   Inactive

\* Factory setting

## 6.2.8.3 Weighing configuration

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Weight capture mode	Defines the behavior when the button to add the result was tapped, or when the add result was triggered by the automatic weighing result creation. <b>Stable:</b> The balance waits for a stable weight. <b>Immediate:</b> The balance does not wait for a stable weight.	Stable*   Immediate

\* Factory setting

### Series / Statistics

Parameter	Description	Values
Measurement series	A measurement series can be performed.	Active   Inactive*
Statistical calculations	Statistical information is provided. This setting is only available if the parameter <b>Measurement series</b> is activated.	Active   Inactive*
Acceptance range	Defines the acceptance range for the statistical calculations. This setting is only available if the parameter Statistical calculations is activated.	Active   Inactive* Numeric (%)

\* Factory setting

## 6.2.8.4 Report configuration

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines which quality information is published.	Adjustment date/time   Level state   MinWeigh state
Task information	Defines which information about the task is published.	Application settings   Measurement details
Result detail information	Defines which information related to the measurement result is published.	Tare / Gross weight   Date/time

## 6.3 Adjustment settings

### See also

 [Editing an adjustment](#) ▶ Page 46

### 6.3.1 Settings: Adjustment strategy

≡ **Navigation:** ▼ >  **Applications** >  **Adjustments** > **inactive adjustment**

Parameter	Description	Values
Adjustment strategy	Defines the type of adjustment to be performed. For approved balances, this setting is not available.	No adjustment   Internal adjustment*   External adjustment

\* Factory setting

### See also

 [Adjustment strategy](#) ▶ Page 46

### 6.3.2 Settings: Internal adjustment

≡ **Navigation:** ▼ >  **Applications** >  **Adjustments** >  **Internal** >  \*

The settings are divided into the following subsections:

-  **Specification**
-  **Report**

#### Specification

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Planning - Start events	Serves to plan after which event an adjustment is automatically executed. Multiple selections are allowed.	Active*   Inactive <ul style="list-style-type: none"> <li>• Start after temperature change</li> <li>• Start after leveling</li> <li>• Start after power-on</li> </ul>

Planning - Schedule	Serves to plan at what time and on which weekday an adjustment is automatically executed. <ul style="list-style-type: none"> <li>• <b>Start time:</b> Up to three start times can be defined.</li> <li>• <b>Preferred days:</b> Monday, Tuesday, ... Sunday</li> </ul>	Active*   Inactive Numeric
---------------------	--	-------------------------------

\* Factory setting

### Report

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines whether the leveling status of the balance is published.	Level state

## 6.3.3 Settings: External adjustment

Navigation: > Applications > Adjustments > External >

The settings are divided into the following subsections:

- Specification
- Report

### Specification

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Nominal weight	Defines the approximate, rounded value of the test weight.	Numeric The available units depend on the balance model.

\* Factory setting

### Report

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines whether the leveling status of the balance is published.	Level state

## 6.4 Test settings

Navigation: > Applications >

The section **Tests** is divided into the following subsections:

- Sensitivity
- Repeatability
- Eccentricity

## 6.4.1 Settings: Sensitivity test

Navigation: Applications > Tests > Sensitivity >

The settings are divided into the following subsections:

- Specification
- Report

### Specification

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Tare container	Defines whether a tare container is used.	Active   Inactive*

\* Factory setting

### Test Point

Up to two test points can be defined.

Parameter	Description	Values
Nominal weight	Defines the nominal value of the weight that is used for the test.	Numeric The available units depend on the balance model.
Control limit	Defines the error tolerance of a process with respect to its set value. Exceeding the value <b>Control limit</b> is a violation of quality requirements and therefore requires a correction of the process. If the value <b>Control limit</b> is exceeded: The test failed, the balance is out of specification.	Numeric The available units depend on the balance model.
Warning limit	Defines the upper or lower limit that, if exceeded or not reached, makes more stringent process monitoring necessary. The value <b>Warning limit</b> must be smaller than the value <b>Control limit</b> . Result if the value <b>Warning limit</b> is exceeded: The test is passed, but the difference is higher than expected.	Active   Inactive* Numeric

\* Factory setting

### Report

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines whether the leveling status of the balance is published.	Level state

## 6.4.2 Settings: Repeatability test

Navigation: Applications > Tests > Repeatability >

The settings are divided into the following subsections:

- Specification
- Report

## Specification

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d
Number of repetitions	Defines the number of weight measurements of a series.	Numeric (10*   4...20)
Tare container	Defines whether a tare container is used.	Active   Inactive*

\* Factory setting

## Test Point

Parameter	Description	Values
Nominal weight	Defines the nominal value of the weight that is used for the test.	Numeric The available units depend on the balance model.
Control limit	Defines the error tolerance of a process with respect to its set value. Exceeding the value <b>Control limit</b> is a violation of quality requirements and therefore requires a correction of the process. If the value <b>Control limit</b> is exceeded: The test failed, the balance is out of specification.	Numeric The available units depend on the balance model.
Warning limit	Defines the upper or lower limit that, if exceeded or not reached, makes more stringent process monitoring necessary. The value <b>Warning limit</b> must be smaller than the value <b>Control limit</b> . Result if the value <b>Warning limit</b> is exceeded: The test is passed, but the difference is higher than expected.	Active   Inactive* Numeric

\* Factory setting

## Report

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines whether the leveling status of the balance is published.	Level state

## See also

[Repeatability test](#) ▶ Page 48

### 6.4.3 Settings: Eccentricity test

☰ **Navigation:** ▼ > ☰ **Applications** > ⚙️ **Tests** > ⚙️ **Eccentricity** > ⚙️

The settings are divided into the following subsections:

- ⚙️ **Specification**
- 📄 **Report**

#### Specification

Parameter	Description	Values
Weighing profile	Defines the weighing profile.	General*   10d

\* Factory setting

## Test Point

Parameter	Description	Values
Nominal weight	Defines the nominal value of the weight that is used for the test.	Numeric The available units depend on the balance model.
Control limit	Defines the error tolerance of a process with respect to its set value. Exceeding the value <b>Control limit</b> is a violation of quality requirements and therefore requires a correction of the process. If the value <b>Control limit</b> is exceeded: The test failed, the balance is out of specification.	Numeric The available units depend on the balance model.
Warning limit	Defines the upper or lower limit that, if exceeded or not reached, makes more stringent process monitoring necessary. The value <b>Warning limit</b> must be smaller than the value <b>Control limit</b> . Result if the value <b>Warning limit</b> is exceeded: The test is passed, but the difference is higher than expected.	Active   Inactive* Numeric

\* Factory setting

## Report

Parameter	Description	Values
Header and Footer	Defines the header and/or the footer to be published.	Title   Date/time   User   Signature   Empty lines
Balance information	Defines which information about the balance is published.	Balance type   Balance ID   Balance serial number   Software version
Quality information	Defines whether the leveling status of the balance is published.	Level state

## See also

[Eccentricity test](#) ▶ Page 49

## 7 Maintenance

To guarantee the functionality of the balance and the accuracy of the weighing results, a number of maintenance actions must be performed by the user.

### 7.1 Maintenance tasks

Maintenance action	Recommended interval	Remarks
Performing an internal or external adjustment	<ul style="list-style-type: none"><li>Daily</li><li>After cleaning</li><li>After leveling</li><li>After changing the location</li></ul>	see "Adjustments"
Performing routine tests (eccentricity test, repeatability test, sensitivity test). METTLER TOLEDO recommends to at least perform a sensitivity test.	<ul style="list-style-type: none"><li>After cleaning</li><li>After assembling the balance</li><li>After a software update</li><li>Depending on your internal regulations (SOP)</li></ul>	see "Tests"
Cleaning	<ul style="list-style-type: none"><li>After every use</li><li>Depending on the degree of pollution</li><li>Depending on your internal regulations (SOP)</li></ul>	see "Cleaning"
Updating the software	<ul style="list-style-type: none"><li>Depending on your internal regulations (SOP).</li><li>After a new software release.</li></ul>	see "Software update"

#### See also

- [Adjustments](#) ▶ Page 46
- [Tests](#) ▶ Page 47
- [Cleaning](#) ▶ Page 99
- [Software update](#) ▶ Page 104

### 7.2 Cleaning

#### 7.2.1 Disassembling for cleaning

##### Note

Depending on the balance model, the components may look different.

##### Note

In most cases, it is not necessary to remove the protective cover to clean the balance.

##### 7.2.1.1 Balances with draft shield




#### CAUTION

##### **Injury due to sharp objects or broken glass**


Instrument components, e.g., glass, can break and lead to injuries.

- Always proceed with focus and care.


- 1 Remove the weighing pan (1) and the drip tray (2).

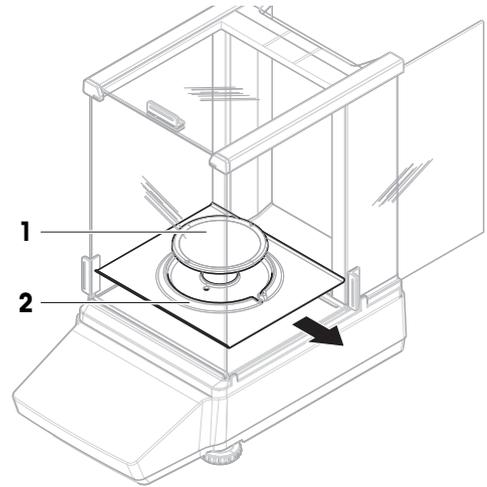


- 2 Turn the QuickLock (3, right, left) and pull the side door (4) towards the front to remove it (right, left).

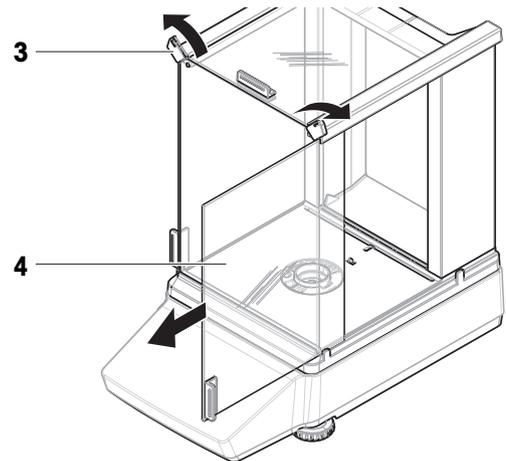

- 3 Tilt the front panel (5) towards the front and lift it upwards to remove it.

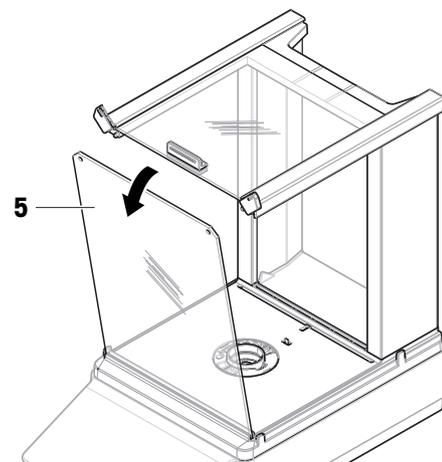


- 4 Pull the top door (6) towards the front to remove it.

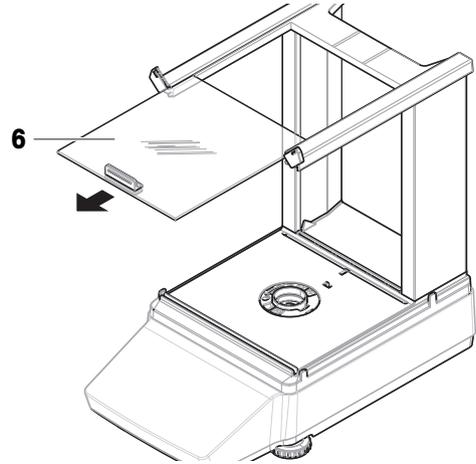


- 5 Press the release button (7) and tilt the back panel (8) to remove it.

**Note**


Optional, if required: Remove the protective cover for cleaning as described below.

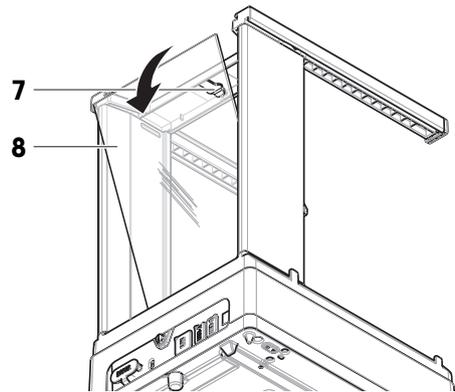

- 6 Open the QuickLock (9) and remove the draft shield (10).

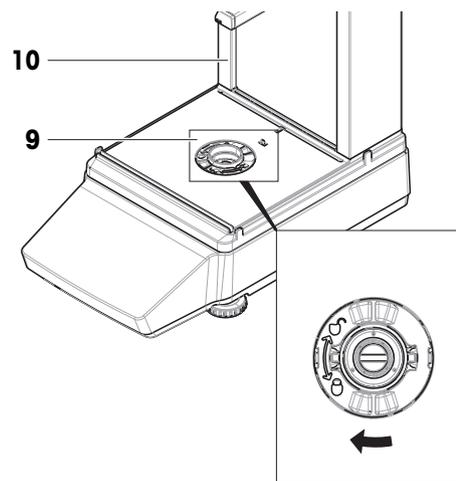

- 7 Remove the protective cover (11) from the weighing platform (12).

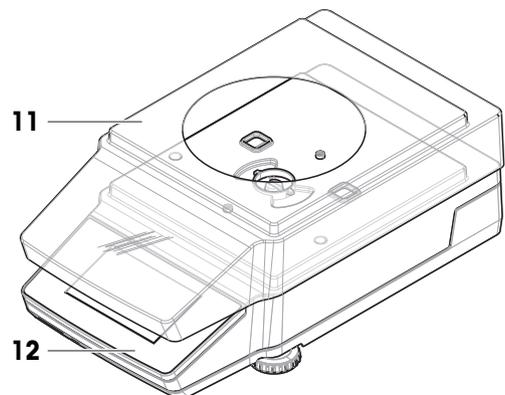


### 7.2.1.2 Balances without draft shield


- 1 Remove the draft-protection element (1).
- 2 Remove the weighing pan (2).
- 3 Remove the weighing pan support (3).

**Note**

Optional, if required: Remove the protective cover for cleaning as described below.

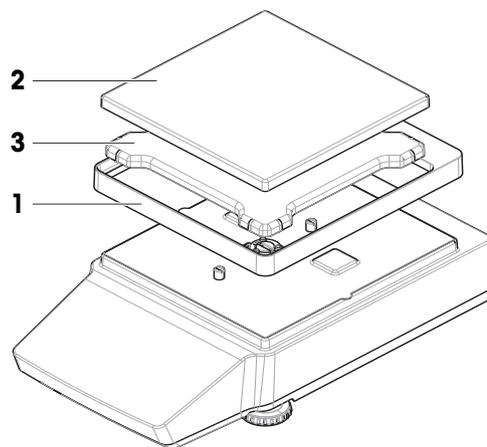

- 4 Remove the screws (4) to remove the EMC plate (5).
- 5 Remove the protective cover (6) from the weighing platform (7).

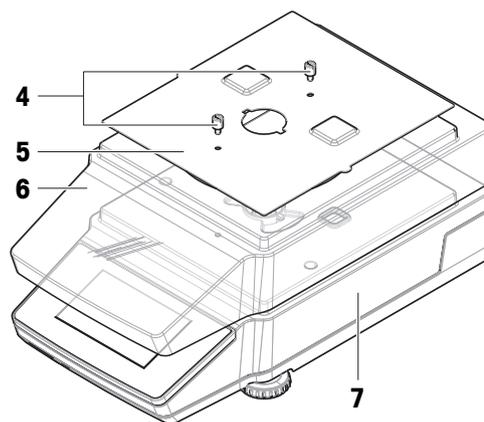

### 7.2.2 Cleaning agents

In the following table, cleaning tools and cleaning agents recommended by METTLER TOLEDO are listed. Pay attention to the concentration of the agents specified in the table.

		Tools				Cleaning agents					
		Paper tissue	Brush	Dishwasher	Water	Acetone	Ethanol (70%)	Isopropanol (70%)	Hydrochloric acid (3-10%)	Sodium hydroxide (0.2-1.0 M)	Peracetic acid (2-3%)
Around the balance	Balance housing	✓	R	—	R	—	R	✓	R	R	R
	Feet	✓	R	—	R	—	R	✓	R	R	R
Balance terminal	Terminal	✓	R	—	✓	PR	R	R	R	R	R
	Display	✓	—	—	✓	PR	R	R	R	R	R
	Terminal cover	✓	R	—	✓	—	R	R	R	PR	PR

		Paper tissue	Brush	Dishwasher	Water	Acetone	Ethanol (70%)	Isopropanol (70%)	Hydrochloric acid (3-10%)	Sodium hydroxide (0.2-1.0 M)	Peracetic acid (2-3%)
Balance draft shield	Glass panels	✓	R	R	R	PR	✓	✓	R	R	R
	Non-removable handles and frames	✓	R	—	R	PR	✓	✓	R	R	R
Weighing area	Weighing pan	R	R	✓	R	R	✓	✓	R	R	R
	Drip tray	R	R	✓	R	R	✓	✓	—	—	R

### Legend

- ✓ Best recommendation by METTLER TOLEDO; can be used without limitation.
- R Recommended by METTLER TOLEDO; can be used without limitation.
- PR Partially recommended by METTLER TOLEDO: individual resistance to acid and alkali must be evaluated, including dependence to the time exposure.
- Not recommend. High risk for damage.

## 7.2.3 Cleaning the balance



### NOTICE

#### Damage to the instrument due to inappropriate cleaning methods

If liquid enters the housing, it can damage the instrument. The surface of the instrument can be damaged by certain cleaning agents, solvents, or abrasives.

- 1 Do not spray or pour liquid on the instrument.
- 2 Only use the cleaning agents specified in the Reference Manual (RM) of the instrument or the guide "8 Steps to a Clean Balance".
- 3 Only use a lightly moistened, lint-free cloth or a tissue to clean the instrument.
- 4 Wipe off any spills immediately.



For further information on cleaning a balance, consult "8 Steps to a Clean Balance".

► [www.mt.com/lab-cleaning-guide](http://www.mt.com/lab-cleaning-guide)

#### Cleaning around the balance

- Remove any dirt or dust around the balance and avoid further contaminations.

#### Cleaning the terminal

- Clean the terminal with a damp cloth or a tissue and a mild cleaning agent.

#### Cleaning the removable parts

- Clean the removed part with a damp cloth or a tissue and a mild cleaning agent or clean in a dishwasher up to 80 °C.

## Cleaning the weighing unit

- 1 Disconnect the balance from the AC/DC adapter.
- 2 Use a lint-free cloth moistened with a mild cleaning agent to clean the surface of the balance.
- 3 Remove powder or dust with a disposable tissue first.
- 4 Remove sticky substances with a damp lint-free cloth and a mild solvent, e.g., isopropanol or ethanol 70%.

### 7.2.4 Putting into operation after cleaning

- 1 Reassemble the balance.
- 2 Check that the draft shield doors (top, sides) open and close normally (if applicable).
- 3 Reconnect the balance to the AC/DC adapter.
- 4 Check the level status, level the balance if necessary.
- 5 Respect the warm-up time specified in the "Technical Data".
- 6 Perform an internal adjustment.
- 7 Perform a routine test according to the internal regulations of your company. METTLER TOLEDO recommends performing a sensitivity test after cleaning the balance.
- 8 Press **→0←** to zero the balance.
  - ➔ The balance is ready for use.

#### See also

- 🔗 Leveling the balance ▶ Page 28
- 🔗 Technical Data ▶ Page 111
- 🔗 Performing an internal adjustment ▶ Page 47

## 7.3 Service

Regular servicing by an authorized service technician ensures reliability for years to come. Contact your METTLER TOLEDO representative for details about the available service options.

## 7.4 Software update

Search for software:

▶ [www.mt.com/labweighing-software-download](http://www.mt.com/labweighing-software-download)

Contact a METTLER TOLEDO service representative if you need support updating the software.

METTLER TOLEDO recommends saving the data on a storage device before updating the software.

### 7.4.1 Updating the software

≡ **Navigation:** ≡ **Balance menu** > ≡ **Maintenance** > 📄 **Software update**

The function **Software update** is only available to users with the corresponding rights.

- A USB storage device containing the software installer is connected to the balance.

- 1 Tap 📄 **Software update**.
- 2 Select **Software update**.
- 3 Tap **→ Next**.
  - ➔ An update wizard opens and leads you step-by-step through the procedure.
- 4 When prompted, tap **I accept the terms in the license agreement** and confirm with **✓ OK**.

### 7.4.2 Putting into operation after software update

- 1 Press **🔌** to switch on the balance.

- 2 Check the level status. Level the balance if required.
- 3 Perform an internal adjustment.
- 4 Perform a routine test according to the internal regulations of your company.
- 5 Press **→0←** to zero the balance.
  - ➔ The balance is ready for use.

#### See also

- [Leveling the balance](#) ▶ Page 28
- [Performing an internal adjustment](#) ▶ Page 47

## 7.5 Resetting the balance

A reset puts the balance back to factory state. All user data are deleted. Resetting the balance requires corresponding permission.



### NOTICE

#### Reset causes data loss

Resetting the balance will delete user application data and set the user configuration back to factory state.

- **User management > General:** The user's configuration permission is activated.
- 1 Tap **☰ Menu**.
- 2 Tap **⚙ Maintenance**.
- 3 Tap **↻ Reset**.
- 4 Tap **↻ Reset** to confirm.
  - ➔ The balance restarts with factory settings.

## 8 Troubleshooting

Possible errors with their cause and remedy are described in the following chapter. If there are errors that cannot be corrected through these instructions, contact METTLER TOLEDO.

### 8.1 Error messages

Error message	Possible cause	Diagnostic	Remedy
The balance shows an error code.	Software or hardware error.	–	Perform a balance reset. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Date and time lost</b>	The battery (capacitor) is low. The battery (capacitor) backup is lost.	Check the settings for date and time.	Connect the balance to the power outlet and let the battery (capacitor) charge for two to three days. Set date and time. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Communication with weighing module is not possible.</b>	The internal communication does not work properly.	–	Perform a balance reset. Reinstall the balance software. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Data memory defect.</b>	EEPROM is corrupt.	–	Perform a balance reset. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Memory full.</b>	The memory storage is full.	–	Perform a balance reset.
<b>No standard adjustment.</b>	The standard adjustment is missing or invalid.	–	Contact your METTLER TOLEDO service representative.
<b>Program memory defect.</b>	The checksum for the stored program is not correct anymore.	–	Reinstall the balance software. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Temperature sensor defect..</b>	The temperature sensor that measures the cell temperature is defective.	–	Contact your METTLER TOLEDO service representative.
<b>Type data damaged.</b>	The TDNR is corrupt.	–	Perform a balance reset. If the issue persists, contact your METTLER TOLEDO service representative.

Error message	Possible cause	Diagnostic	Remedy
<b>Unexpected startup problem</b>	A problem occurred while starting up the balance. Some data could not be read correctly from the memory.	–	Restart the balance. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Unknown error</b>	General error for an unspecific issue.	–	Restart the balance. Perform a balance reset. If the issue persists, contact your METTLER TOLEDO service representative.
<b>User data damaged.</b>	The user data is damaged or its context is incorrect.	–	Perform a balance reset. If the issue persists, contact your METTLER TOLEDO service representative.
<b>Wrong cell data.</b>	The cell data is damaged or its checksum is incorrect.	–	Contact your METTLER TOLEDO service representative.
<b>Wrong legally relevant authentication.</b> Only applies to approved balances.	–	–	Contact your METTLER TOLEDO service representative.

## 8.2 Error symptoms

Error symptom	Possible cause	Diagnostic	Remedy
The balance shows no valid date and time.	The battery (capacitor) is low. The battery (capacitor) backup is lost.	Check the settings for date and time.	Connect the balance to the power outlet and let the battery (capacitor) charge for two to three days. Set date and time. If the issue persists, contact your METTLER TOLEDO service representative.
The display is dark.	The balance is on standby or in power-saving mode.	–	Switch on the balance.
	There is no power.	Check the connection to the AC/DC adapter and the power outlet.	Connect the balance to the power outlet. See "Connecting the balance".
	The wrong AC/DC adapter is connected to the balance.	Check the AC/DC adapter, see "Technical Data".	Use the correct AC/DC adapter.
	The AC/DC adapter is defective.	–	Replace the AC/DC adapter.
	The display is defective.	–	Contact your METTLER TOLEDO service representative.

Error symptom	Possible cause	Diagnostic	Remedy
The balance does not react to any input.	Software freeze.	–	Disconnect the power cable from the balance and reconnect it after a few seconds. Perform a balance reset. If the issue persists, contact your METTLER TOLEDO service representative.
The balance does not start up properly.	The balance has not power.	Check if the AC/DC adapter is plugged in.	Connect the AC/DC adapter.
	The AC/DC adapter is defective.	Check with another AC/DC adapter if available.	Replace the AC/DC adapter, see accessories list.
The balance does not return to zero the weight is removed.	Something is touching the weighing pan. Dirt or dust on the weighing pan.	Remove the weighing pan and check it for dirt or dust.	Clean the weighing pan. If the issue persists, contact your METTLER TOLEDO service representative.
Taring fails.	The weighing bench is vibrating.	Tab →← and check if the value on the display is still unstable.	Place the balance on a weighing bench free of vibrations.
	The weighing sample is electrostatically charged.	Place a test weight on the weighing pan. Check if the weighing result is stable.	For balances with a draft shield: place a water container into the weighing chamber to increase the humidity. Use an antistatic device, see accessories list.
The internal adjustment fails.	A weight is on the weighing pan.	–	Remove the weight from the weighing pan.
	Repeatability is poor.	–	Perform a repeatability test.
	The internal weight does not function properly.	–	Contact your METTLER TOLEDO service representative.
The sensitivity test fails.	A weight is on the weighing pan.	–	Remove the weight from the weighing pan.
	The internal weight does not work properly.	–	Contact your METTLER TOLEDO service representative.
The repeatability test fails.	Eccentricity is out of tolerance.	Perform an eccentricity test.	If the eccentricity test fails, contact your METTLER TOLEDO service representative.
	The environment is unstable.	–	Place the balance in a location with suitable environmental conditions.

<b>Error symptom</b>	<b>Possible cause</b>	<b>Diagnostic</b>	<b>Remedy</b>
The display shows overload or underload.	The wrong weighing pan is installed.	Slightly lift or press the weighing pan to see if the weight appears on the display.	Install a proper weighing pan.
	No weighing pan is installed.	–	Install a proper weighing pan.
	Incorrect zero point when the balance is switched on.	–	Disconnect the power cable and reconnect it after a few seconds.
	The balance is not adjusted.	–	Perform an internal adjustment. See section "Performing an internal adjustment".
The value on the display oscillates.	Vibrations on the weighing bench, for example, building vibrations, foot traffic.	Place a beaker with water on the weighing bench. Vibrations cause ripples on the water surface.	Protect the weighing location against vibrations, for example, with an absorber. Find a different weighing location.
	Draft due to untight draft shield and/or open window.	Check the draft shield for gaps.	Fix the draft shield. Close the window.
	The weighing sample is electrostatically charged.	Check if the weighing result is stable when using a test weight.	Increase the air humidity in the weighing chamber. Use an ionizer. See "Accessories".
	The location is not suitable for weighing.	–	Follow the requirements for the location. See "Selecting the location".
	Something is touching the weighing pan.	Check for touching parts or dirt.	Remove touching parts. Clean the balance.
The value on the display is drifting towards plus or minus.	The location is not suitable for weighing.	–	Place the balance in a location with suitable environmental conditions.
	The weighing sample absorbs moisture or evaporates moisture.	Check if the weighing result is stable when using a test weight.	Cover the weighing sample.
	The weighing sample is electrostatically charged.	Use a test weight to check if the weighing result is stable.	Increase the humidity in the weighing chamber. Use an ionizer, see accessories list.
	The weighing sample is warmer or colder than the air in the weighing chamber.	Check if the weighing result is stable when using an acclimatized test weight.	Bring the sample to room temperature.
	The balance has not yet warmed up.	–	Let the balance warm up. Adequate warm-up time is specified in the section "General data".

### 8.3 Saving a support file

When requesting help from your METTLER TOLEDO service representative, you may be asked to send a support file. This file is analyzed and can help to solve issues with the balance.

≡ **Navigation:** ≡ **Balance menu** > ≡ **Maintenance**

- The section ≡ **Maintenance** is open.
- A USB storage device is available.
- 1 Tap ≡ **Save support file**.
- 2 Connect a USB storage device to the balance.
- 3 Tap ✓ **OK**.
  - ➔ The support file is saved to the USB storage device.

### 8.4 Putting into operation after fixing an error

After troubleshooting, perform the following steps to put the balance into operation:

- Ensure that the balance is completely reassembled and cleaned.
- Reconnect the balance to the AC/DC adapter.

## 9 Technical Data

### 9.1 General data

#### Power supply

AC/DC adapter:	Input: 100 – 240 V AC $\pm$ 10%, 50 – 60 Hz, 0.5 A Output: 12 V DC, 1 A, LPS
Balance power consumption:	12 V DC, 0.8 A
Polarity:	

#### Protection and standards

Overvoltage category:	II
Degree of pollution:	2
Ingress protection code:	IP43 (balances with readability of 10 mg or higher)

#### Note

Stated IP is only achieved when the balance is ready for operation. The protective cover must be installed, and the caps must cover the interface connections.

Standards for safety and EMC:	See Declaration of Conformity
Range of application:	Use only indoors in dry locations

#### Environmental conditions

The limit values apply when the balance is used under the following environmental conditions:

Height above mean sea level:	Up to 5000 m
Ambient temperature:	+10 – +30 °C
Temperature change, max.:	5 °C/h
Relative humidity:	30 – 70%, non-condensing
Acclimatization time:	Recommendation: Up to <b>4 hours</b> for precision balances, or up to <b>8 hours</b> for analytical balances. These values apply after placing the balance in the same location where it will be put into operation.

#### Note

The acclimatization time depends on the readability of the balance, and on the environmental conditions.

Warm-up time:	At least <b>30 minutes</b> for precision balances, or <b>60 minutes</b> for analytical balances. These values apply after connecting the balance to the power supply, or after exiting power-saving mode. When switched on from standby, the balance is ready for operation immediately.
---------------	--

The balance can be used under the following environmental conditions. However, the weighing performances of the balance may be outside the limit values:

Ambient temperature:	+5 °C – +40 °C
Relative humidity:	20% to max. 80% at 31 °C, decreasing linearly to 50% at 40 °C, non-condensing

The balance can be disconnected and stored in its packaging under the following conditions:

Ambient temperature:	-25 – +70 °C
Relative humidity:	10 – 90%, non-condensing

## 9.2 Model-specific data

### 9.2.1 Analytical balances, readability 0.1 mg

	MR104	MR204	MR304
<b>Limit values</b>			
Capacity	120 g	220 g	320 g
Nominal load	100 g	200 g	300 g
Readability	0.1 mg	0.1 mg	0.1 mg
Repeatability (at 5% load)	0.1 mg	0.1 mg	0.1 mg
Linearity deviation	0.2 mg	0.2 mg	0.2 mg
Eccentricity deviation (at test load)	0.4 mg (50 g)	0.4 mg (100 g)	0.4 mg (100 g)
Sensitivity offset (at nominal load) ▲	0.5 mg	0.8 mg	1 mg
Sensitivity temperature drift	0.0002%/°C	0.0002%/°C	0.0002%/°C
<b>Typical values</b>			
Repeatability (at 5% load)	0.08 mg	0.08 mg	0.08 mg
Linearity deviation	0.06 mg	0.06 mg	0.06 mg
Eccentricity deviation (at test load)	0.12 mg (50 g)	0.12 mg (100 g)	0.12 mg (100 g)
Sensitivity offset (at nominal load) ▲	0.3 mg	0.5 mg	0.6 mg
Minimum weight (USP, tolerance = 0.10%) ▼	160 mg	160 mg	160 mg
Minimum weight (tolerance = 1%) ▼	16 mg	16 mg	16 mg
Settling time	2 s	2 s	2 s
<b>Dimensions and other specifications</b>			
Balance dimensions (W × D × H)	209 × 351 × 354 mm	209 × 351 × 354 mm	209 × 351 × 354 mm
Weighing pan diameter	90 mm	90 mm	90 mm
Usable height of draft shield	238 mm	238 mm	238 mm
Balance weight	6.4 kg	6.4 kg	6.4 kg
<b>Weights for routine testing</b>			
Weights (OIML class)	100 g (F2) / 5 g (F2)	200 g (F2) / 10 g (F2)	200 g (F2) / 10 g (F2)
Weights (ASTM class)	100 g (ASTM 1) / 5 g (ASTM 1)	200 g (ASTM 1) / 10 g (ASTM 1)	200 g (ASTM 1) / 10 g (ASTM 1)

▲ after adjustment with internal weight

▼ determined at 5% load, k = 2

## 9.2.2 Precision balances, readability 1 mg

	MR203	MR303	MR503	MR603
<b>Limit values</b>				
Capacity	220 g	320 g	520 g	620 g
Nominal load	200 g	300 g	500 g	600 g
Readability	1 mg	1 mg	1 mg	1 mg
Repeatability (at 5% load)	1 mg	1 mg	1 mg	1 mg
Linearity deviation	2 mg	2 mg	2 mg	2 mg
Eccentricity deviation (at test load)	4 mg (100 g)	4 mg (100 g)	4 mg (200 g)	4 mg (200 g)
Sensitivity offset (at nominal load) ▲	8 mg	8 mg	8 mg	8 mg
Sensitivity temperature drift	0.0003%/°C	0.0003%/°C	0.0003%/°C	0.0003%/°C
<b>Typical values</b>				
Repeatability (at 5% load)	0.7 mg	0.7 mg	0.7 mg	0.7 mg
Linearity deviation	0.6 mg	0.6 mg	0.6 mg	0.6 mg
Eccentricity deviation (at test load)	1.2 mg (100 g)	1.2 mg (100 g)	1.2 mg (200 g)	1.2 mg (200 g)
Sensitivity offset (at nominal load) ▲	5 mg	5 mg	5 mg	5 mg
Minimum weight (USP, tolerance = 0.10%) ▼	1.4 g	1.4 g	1.4 g	1.4 g
Minimum weight (tolerance = 1%) ▼	140 mg	140 mg	140 mg	140 mg
Settling time	1.5 s	1.5 s	1.5 s	1.5 s
<b>Dimensions and other specifications</b>				
Balance dimensions (W × D × H)	209 × 351 × 354 mm			
Weighing pan diameter	120 mm	120 mm	120 mm	120 mm
Usable height of draft shield	236 mm	236 mm	236 mm	236 mm
Balance weight	6.5 kg	6.5 kg	6.5 kg	6.5 kg
<b>Weights for routine testing</b>				
Weights (OIML class)	200 g (F2) / 10 g (F2)	200 g (F2) / 10 g (F2)	500 g (F2) / 20 g (F2)	500 g (F2) / 20 g (F2)
Weights (ASTM class)	200 g (ASTM 1) / 10 g (ASTM 1)	200 g (ASTM 1) / 10 g (ASTM 1)	500 g (ASTM 1) / 20 g (ASTM 1)	500 g (ASTM 1) / 20 g (ASTM 1)

▲ after adjustment with internal weight

▼ determined at 5% load, k = 2

### 9.2.3 Precision balances, readability 10 mg or 100 mg

	MR1002	MR2002	MR3002
<b>Limit values</b>			
Capacity	1.2 kg	2.2 kg	3.2 kg
Nominal load	1 kg	2 kg	3 kg
Readability	10 mg	10 mg	10 mg
Repeatability (at 5% load)	10 mg	10 mg	10 mg
Linearity deviation	20 mg	20 mg	20 mg
Eccentricity deviation (at test load)	30 mg (500 g)	30 mg (1 kg)	40 mg (1 kg)
Sensitivity offset (at nominal load) ▲	60 mg	80 mg	80 mg
Sensitivity temperature drift	0.0003%/°C	0.0003%/°C	0.0003%/°C
<b>Typical values</b>			
Repeatability (at 5% load)	7 mg	7 mg	7 mg
Linearity deviation	6 mg	6 mg	6 mg
Eccentricity deviation (at test load)	10 mg (500 g)	10 mg (1 kg)	12 mg (1 kg)
Sensitivity offset (at nominal load) ▲	40 mg	50 mg	50 mg
Minimum weight (USP, tolerance = 0.10%) ▼	14 g	14 g	14 g
Minimum weight (tolerance = 1%) ▼	1.4 g	1.4 g	1.4 g
Settling time	1 s	1 s	1 s
<b>Dimensions and other specifications</b>			
Balance dimensions (W × D × H)	209 × 351 × 100 mm	209 × 351 × 100 mm	209 × 351 × 100 mm
Weighing pan dimensions (W × D)	180 × 180 mm	180 × 180 mm	180 × 180 mm
Balance weight	4.9 kg	4.9 kg	4.9 kg
<b>Weights for routine testing</b>			
Weights (OIML class)	1000 g (F2) / 50 g (F2)	2000 g (F2) / 100 g (F2)	2000 g (F2) / 100 g (F2)
Weights (ASTM class)	1000 g (ASTM 1) / 50 g (ASTM 1)	2000 g (ASTM 1) / 100 g (ASTM 1)	2000 g (ASTM 1) / 100 g (ASTM 1)

▲ after adjustment with internal weight

▼ determined at 5% load, k = 2

	MR4002	MR6002	MR6001
<b>Limit values</b>			
Capacity	4.2 kg	6.2 kg	6.2 kg
Nominal load	4 kg	6 kg	6 kg
Readability	10 mg	10 mg	100 mg
Repeatability (at 5% load)	10 mg	10 mg	80 mg
Linearity deviation	20 mg	20 mg	60 mg
Eccentricity deviation (at test load)	40 mg (2 kg)	40 mg (2 kg)	300 mg (2 kg)
Sensitivity offset (at nominal load) ▲	80 mg	80 mg	300 mg
Sensitivity temperature drift	0.0003%/°C	0.0003%/°C	0.0005%/°C
<b>Typical values</b>			
Repeatability (at 5% load)	7 mg	7 mg	50 mg
Linearity deviation	6 mg	6 mg	20 mg
Eccentricity deviation (at test load)	12 mg (2 kg)	12 mg (2 kg)	100 mg (2 kg)
Sensitivity offset (at nominal load) ▲	50 mg	50 mg	150 mg
Minimum weight (USP, tolerance = 0.10%) ▼	14 g	14 g	100 g
Minimum weight (tolerance = 1%) ▼	1.4 g	1.4 g	10 g
Settling time	1 s	1 s	1 s
<b>Dimensions and other specifications</b>			
Balance dimensions (W × D × H)	209 × 351 × 100 mm	209 × 351 × 100 mm	209 × 351 × 100 mm
Weighing pan dimensions (W × D)	180 × 180 mm	180 × 180 mm	180 × 180 mm
Balance weight	4.9 kg	4.9 kg	4.9 kg
<b>Weights for routine testing</b>			
Weights (OIML class)	2000 g (F2) / 200 g (F2)	5000 g (F2) / 200 g (F2)	5000 g (F2) / 200 g (F2)
Weights (ASTM class)	2000 g (ASTM 4) / 200 g (ASTM 4)	5000 g (ASTM 4) / 200 g (ASTM 4)	5000 g (ASTM 4) / 200 g (ASTM 4)

▲ after adjustment with internal weight


▼ determined at 5% load, k = 2

### 9.3 Dimensions

Dimensions in mm.

#### 9.3.1 MR analytical balances, readability 0.1 mg


Balance models: MR104, MR204, MR304

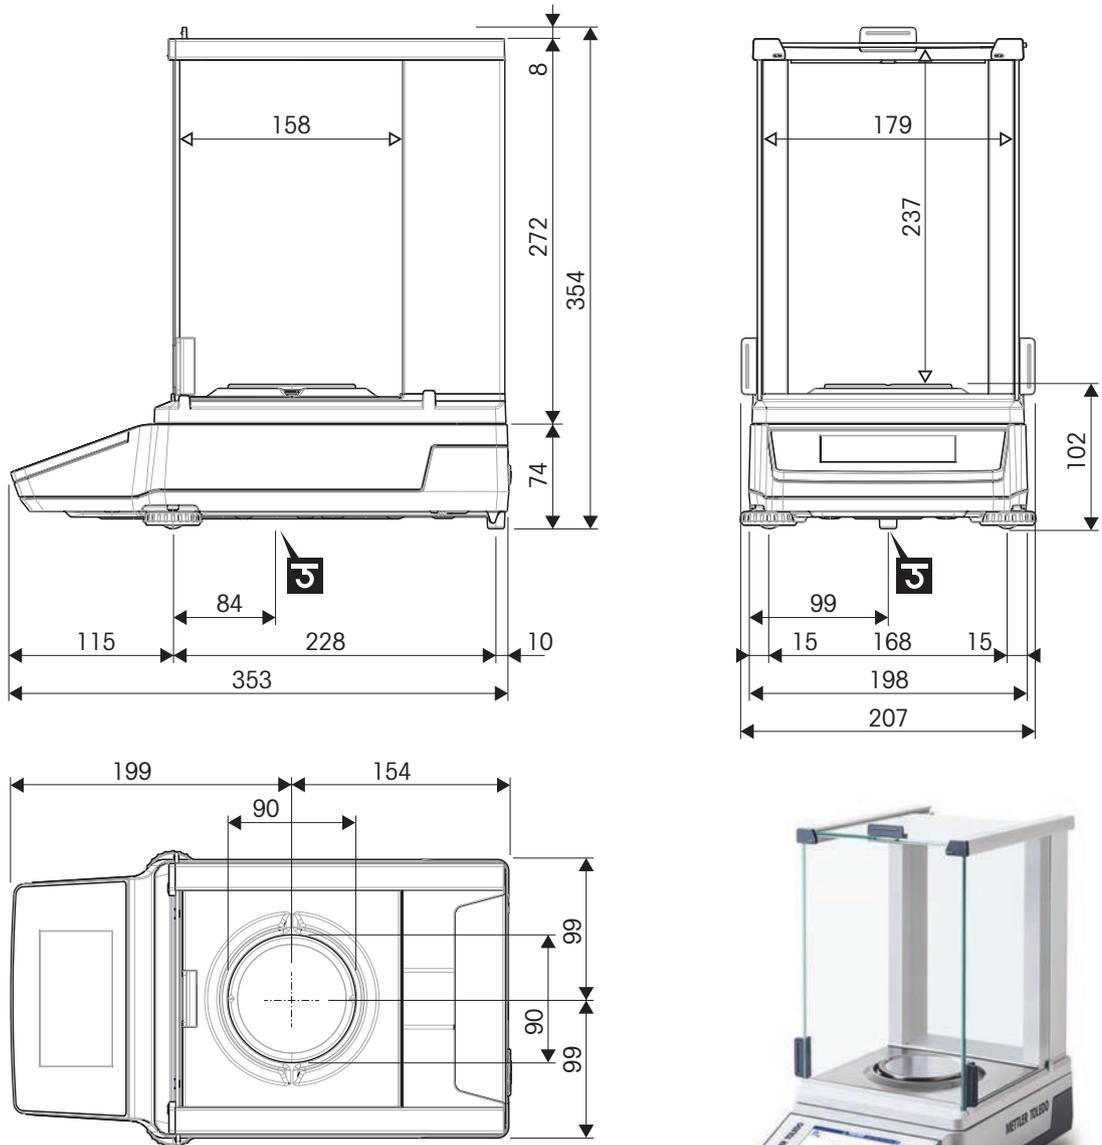

	Outer dimensions [mm]
	Clear dimensions [mm]
	Position of the weighing hook axle

### 9.3.2 MR precision balances, readability 1 mg


Balance models: MR203, MR303, MR503, MR603

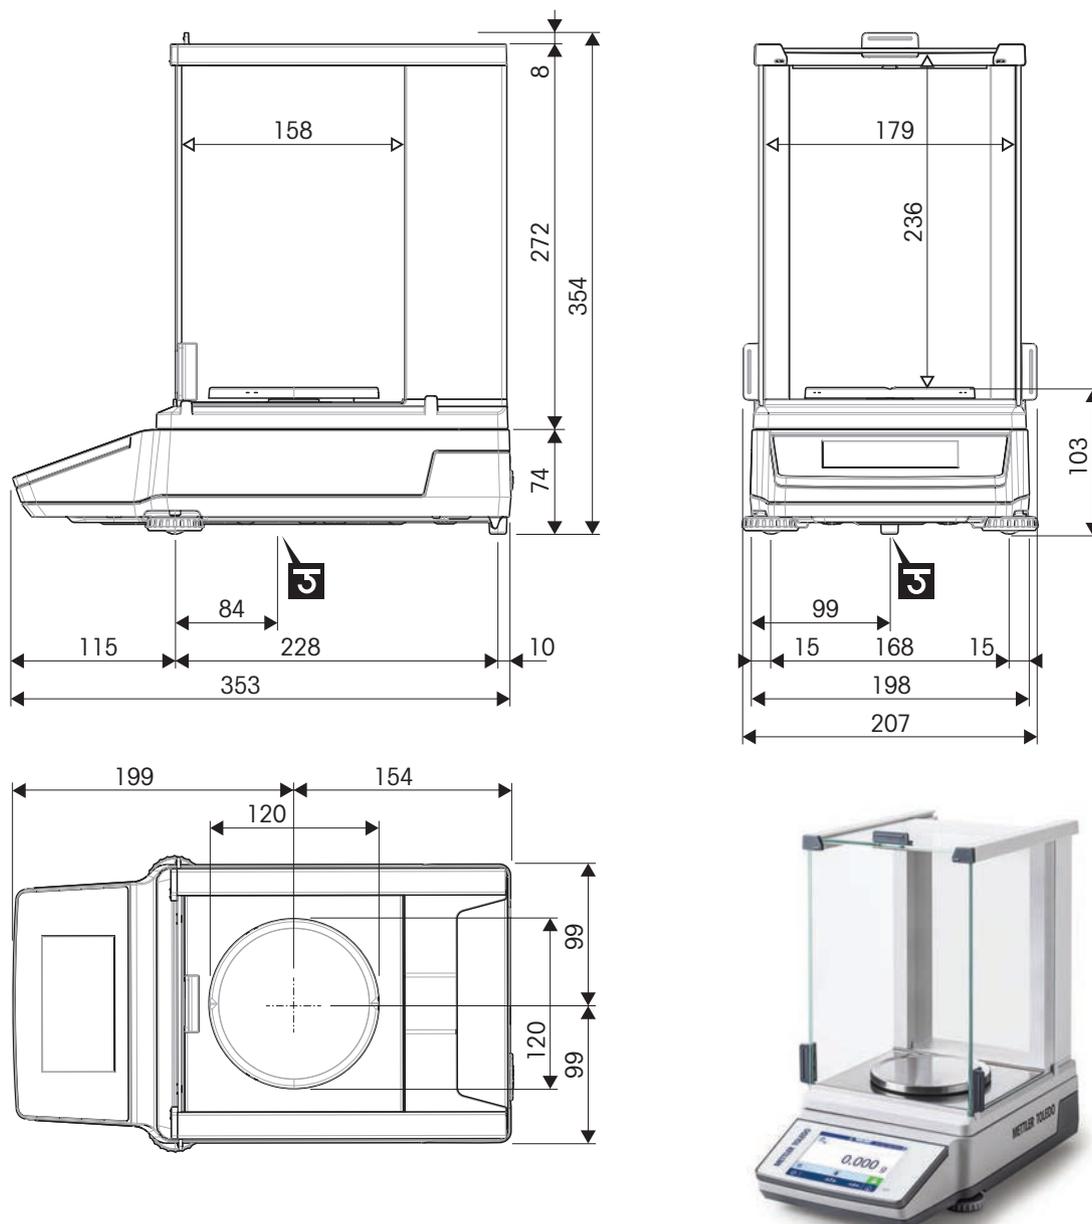

	Outer dimensions [mm]
	Clear dimensions [mm]
	Position of the weighing hook axle

### 9.3.3 MR precision balances, readability 10 mg / 100 mg

Balance models: MR1002, MR2002, MR3002, MR4002, MR6002, MR6001

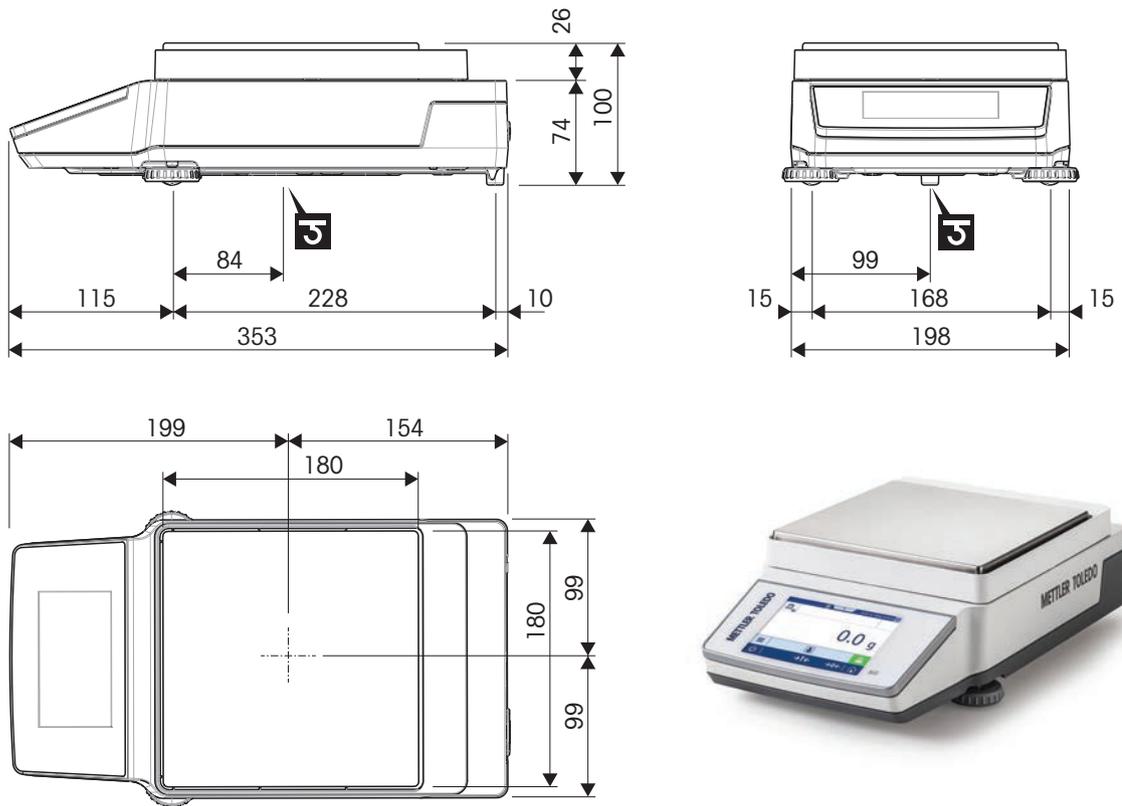

	Outer dimensions [mm]
	Clear dimensions [mm]
<b>J</b>	Position of the weighing hook axle

## 10 Accessories and Spare Parts

### 10.1 Accessories

Accessories are additional components that could help you in your workflow.

#### Antistatic kits

	<b>Antistatic kit universal</b> <span style="float: right;"><b>63052302</b></span> <ul style="list-style-type: none"><li>• Removes electrostatic charges from weighing samples and tare containers</li><li>• Including: U-electrode large (with installation instructions), high-voltage power supply (with user manual and country-specific power cable)</li></ul>
	<b>High-voltage power supply</b> <span style="float: right;"><b>11107766</b></span> <ul style="list-style-type: none"><li>• Supplies up to 2 U-electrodes</li><li>• Including: country-specific power cable, user manual</li><li>• Compatible with: U-electrode large, U-electrode small</li></ul>
	<b>U-electrode large</b> <span style="float: right;"><b>11107764</b></span> <ul style="list-style-type: none"><li>• Removes electrostatic charges from weighing samples and tare containers</li><li>• High-voltage cable with capacitively coupled connector</li></ul>
	<b>U-electrode small</b> <span style="float: right;"><b>11140161</b></span> <ul style="list-style-type: none"><li>• Removes electrostatic charges from weighing samples and tare containers</li><li>• High-voltage cable with capacitively coupled connector</li></ul>
	<b>Ionizer ASK350</b> <span style="float: right;"><b>30893023</b></span> <ul style="list-style-type: none"><li>• Removes small electrostatic charges from weighing samples and tare containers</li></ul>

## Density determination



### Density kit

30706714

- Gravimetric density determination of solids



### Thermometer, calibrated

11132685

- Including: holder, calibration certificate
- For usage in density determination

## Auxiliary displays



### Auxiliary display AD-RS-M7

12122381

- Duplicates the information of the balance display
- Interface: RS232

## Printers



### Printer RS-P25

30702967

- Printing technology: dot matrix



### Printer USB-P25

30702998

- Printing technology: dot matrix



### Printer P-52RUE

30237290

- Printing technology: dot matrix



---

**Printing paper roll, self-adhesive, dot matrix****11600388**

- Set of 3 rolls
- Compatible with: dot matrix printers



---

**Printing paper roll, standard, dot matrix****72456**

- Set of 5 rolls
- Compatible with: dot matrix printers



---

**Ribbon cartridge****65975**

- Including: 2 pcs
- Compatible with: dot matrix printers

---

**Anti-theft devices**

---

**Anti-theft cable****11600361**

---

**Hands-free accessories**

---

**Foot switch****30312558**

- Hands-free taring, zeroing, printing

---


**Barcode readers**

---

**Barcode reader 1D Gryphon GD4220****30417466**

- Scans barcodes and transmits the decoded information to a connected device
- Interface: USB-A

## Cables

	<b>Cable USB-A (f) – USB-C (m)</b> • Data transfer between instrument and USB-A peripheral • Length: 0.16 m	<b>30893021</b>
	<b>USB-C (m) – USB-A (m)</b> • Data transfer between instrument and PC • Length: 1 m	<b>30893022</b>
	<b>Cable RS232 (f) – USB-A (m)</b> • Data transfer between balance and peripheral • Length: 1.7 m	<b>30576241</b>
	<b>Cable RS232 (m) – USB-A (m)</b> • Data transfer between balance and peripheral • Length: 2 m	<b>64088427</b>
	<b>Cable RS9 (m) – RS9 (f)</b> • Data transfer between instrument and peripheral • Length: 1 m	<b>11101051</b>

## Wireless interfaces

	<b>Bluetooth adapter ADP-BT-S, single</b> • Creates a bluetooth connection between instrument and peripheral	<b>30086494</b>
	<b>Bluetooth/Wi-Fi combi adapter LM842</b> • Creates a Bluetooth/Wi-Fi connection between instrument and peripheral	<b>30893006</b>
	<b>Bluetooth/Wi-Fi combi adapter LM842, US</b> • Creates a Bluetooth/Wi-Fi connection between instrument and peripheral	<b>30893005</b>

## Software



EasyDirect Balance

### EasyDirect Balance, 10 licenses

**30540473**

- Data management software for up to 10 balances
- Collection, analysis, storage and export of weighing data



EasyDirect Balance

### EasyDirect Balance, 3 licenses

**30539323**

- Data management software for up to 3 balances
- Collection, analysis, storage and export of weighing data

## Adjustment weights



### Weights

- For routine testing and calibration of weighing instruments
- Available in different accuracy classes
- With calibration certificate (OIML/ASTM)

▶ [www.mt.com/weights](http://www.mt.com/weights)

## Various



### EasyHub USB

**30468768**

- Connects up to 4 peripherals
- Interface to host: USB-B



### SmartPrep weighing funnel

**30061260**

- For weighing powdery substances
- Including: 50 pcs



### Protective foil

**30706721**


- Protects the weighing pan
- Including: 10 pcs

## 10.2 Spare parts

Spare parts are parts that are delivered with the original instrument but that can be replaced, if needed, without the help of a service technician.


### 10.2.1 MR analytical balances, readability 0.1 mg

Balance models: MR104, MR204

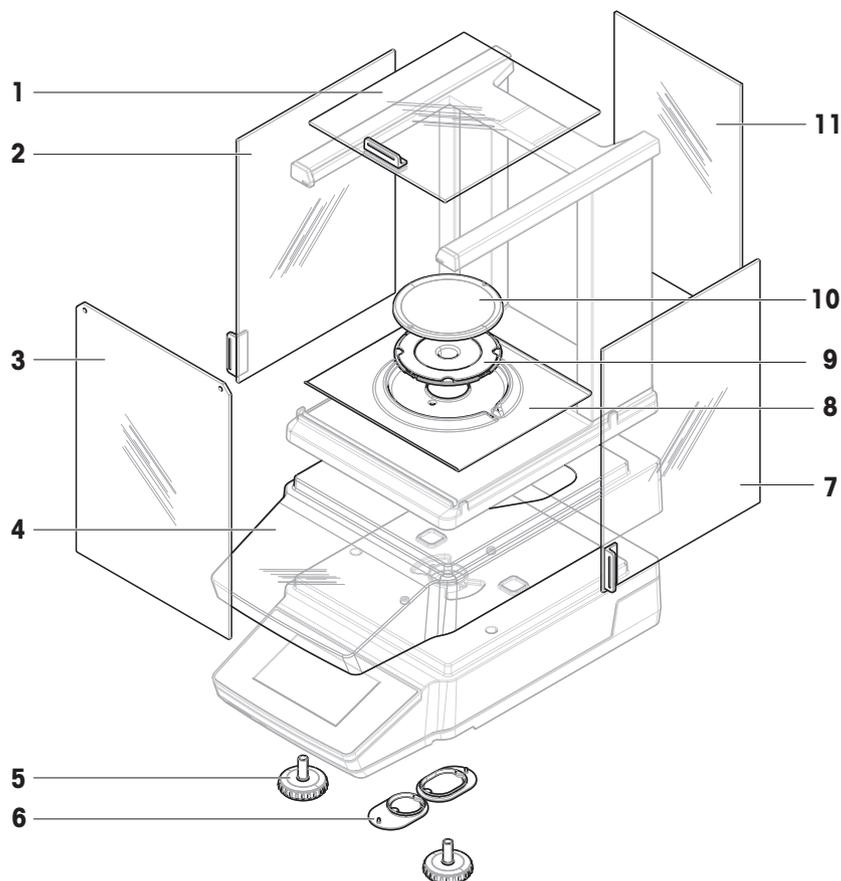

	Order no.	Designation	Remarks
1	30706623	Door, top	Material: glass; including: door handle
2	30706624	Door, left	Material: glass; including: door handle
3	30706626	Panel, front	Material: glass
4	30706656	Protective cover	–
5	30706696	Leveling foot	Including: 2 pcs
6	30706724	Cover, weighing hook	Including: 1 round cover, 1 oval cover; material: silicone
7	30706625	Door, right	Material: glass; including: door handle
8	30706629	Draft-protection element	For weighing pan $\varnothing$ 90 mm
9	30706639	Pan support $\varnothing$ 90 mm	–
10	12122010	Weighing pan $\varnothing$ 90 mm	Excluding: Pan support
11	30706627	Panel, back	Material: glass


Balance model: MR304

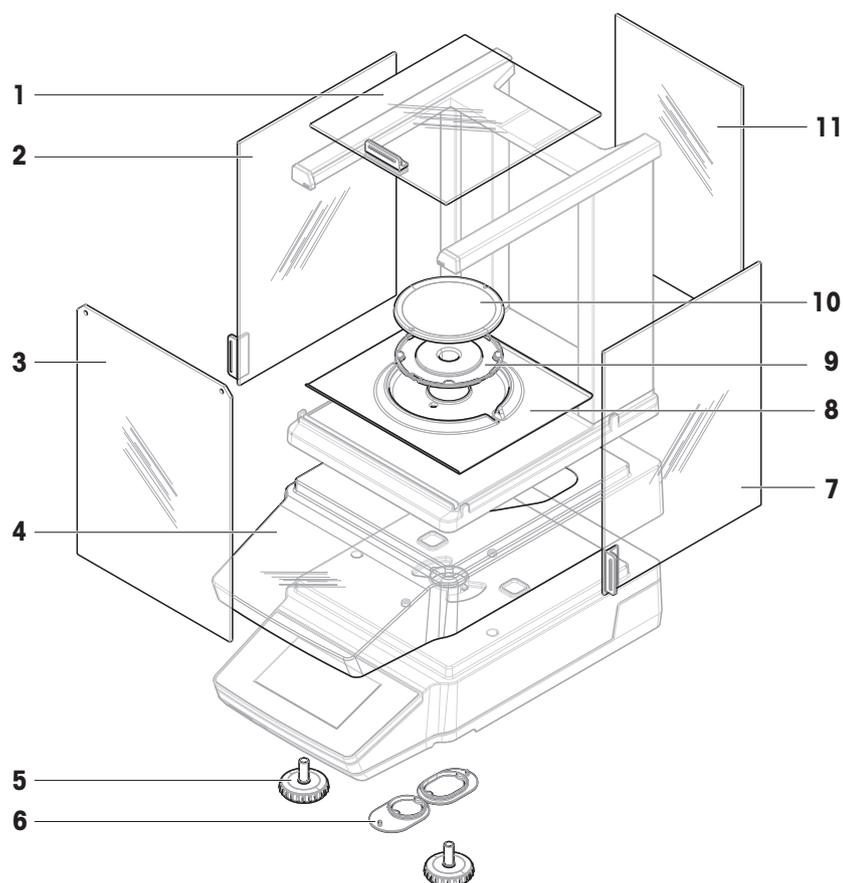

	Order no.	Designation	Remarks
1	30706623	Door, top	Material: glass; including: door handle
2	30706624	Door, left	Material: glass; including: door handle
3	30706626	Panel, front	Material: glass
4	30706656	Protective cover	–
5	30706696	Leveling foot	Including: 2 pcs
6	30706724	Cover, weighing hook	Including: 1 round cover, 1 oval cover; material: silicone
7	30706625	Door, right	Material: glass; including: door handle
8	30706629	Draft-protection element	For weighing pan $\varnothing$ 90 mm
9	30706565	Pan support $\varnothing$ 90 mm	–
10	12122010	Weighing pan $\varnothing$ 90 mm	Excluding: Pan support
11	30706627	Panel, back	Material: glass

## 10.2.2 MR precision balances, readability 1 mg


Balance models: MR203, MR303, MR503, MR603

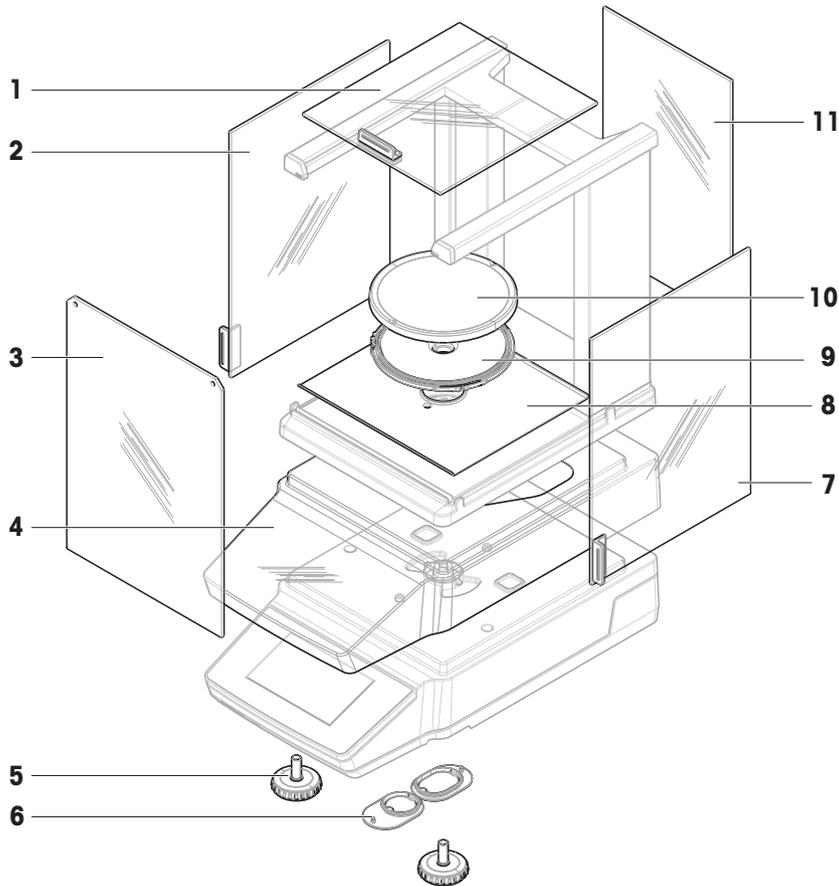

	Order no.	Designation	Remarks
1	30706623	Door, top	Material: glass; including: door handle
2	30706624	Door, left	Material: glass; including: door handle
3	30706626	Panel, front	Material: glass
4	30706656	Protective cover	–
5	30706696	Leveling foot	Including: 2 pcs
6	30706724	Cover, weighing hook	Including: 1 round cover, 1 oval cover; material: silicone
7	30706625	Door, right	Material: glass; including: door handle
8	30850022	Base plate	–
9	30706638	Pan support $\varnothing$ 120 mm	–
10	12122037	Weighing pan $\varnothing$ 120 mm	Excluding: pan support
11	30706627	Panel, back	Material: glass

### 10.2.3 MR precision balances, readability 10 mg / 100 mg


Balance models: MR1002, MR2002, MR3002, MR4002, MR6002, MR6001

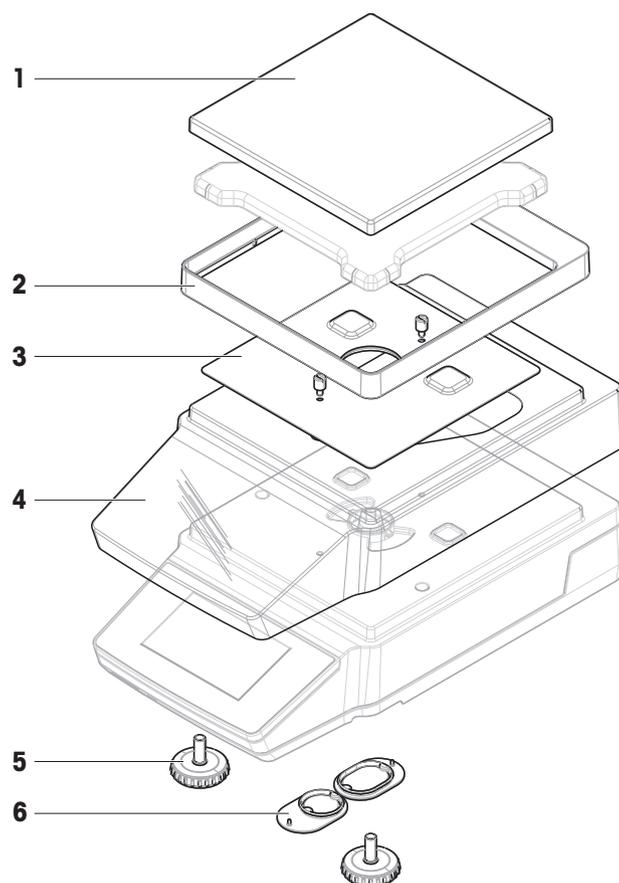

	Order no.	Designation	Remarks
<b>1</b>	30535713	Weighing pan 180 x 180 mm	Excluding: pan support
<b>2</b>	30706647	Draft protection element	–
<b>3</b>	30706650	EMC plate	Including: 2 screws
<b>4</b>	30706657	Protective cover	–
<b>5</b>	30706696	Leveling foot	Including: 2 pcs
<b>6</b>	30706724	Cover, weighing hook	Including: 1 round cover, 1 oval cover; material: silicone

## 10.2.4 AC/DC adapter, universal


Compatible with all MR balance models.

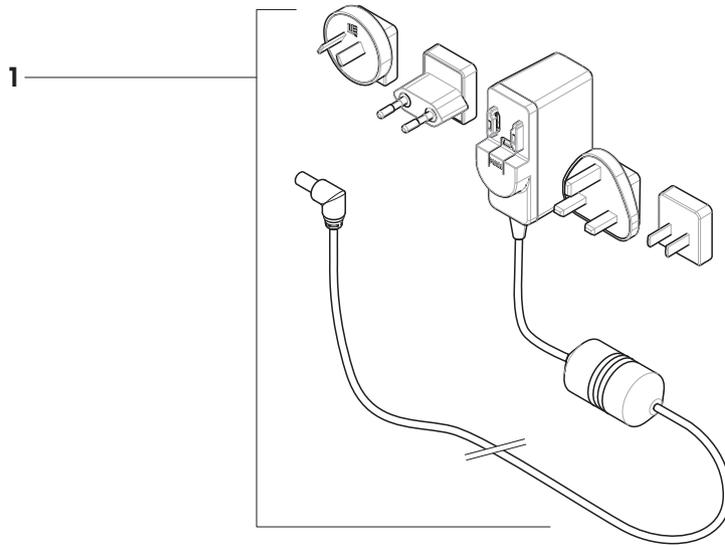

	Order no.	Designation	Remarks
1	30850040	AC/DC adapter universal	Output: 12 V, 1.0 A; including: 4 plugs (EU, UK, US, AU, CN, KR)


## 10.2.5 Packaging

### 10.2.5.1 Balances with draft shield

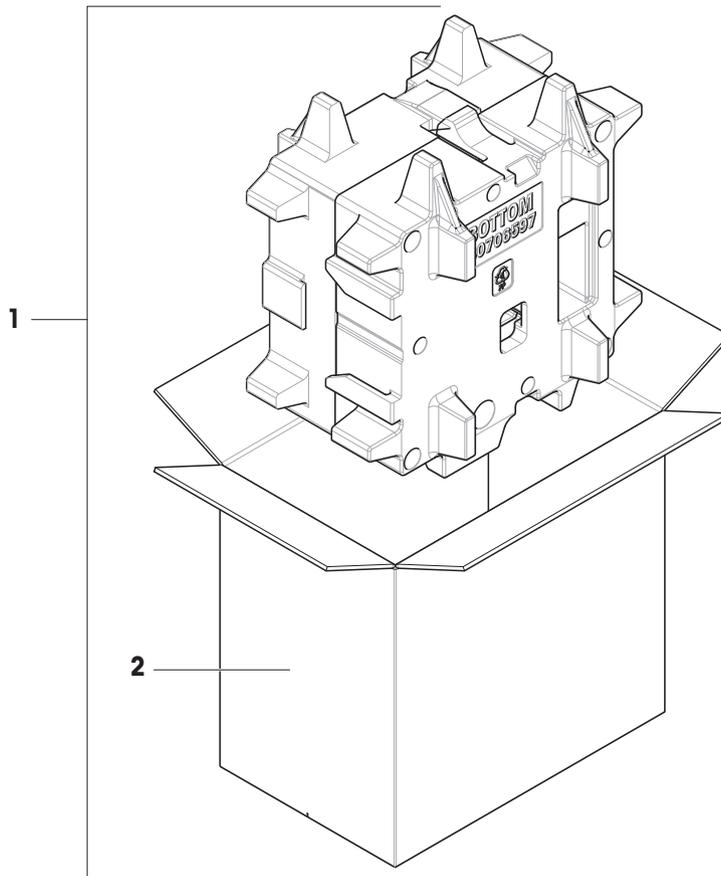

	<b>Order no.</b>	<b>Designation</b>	<b>Remarks</b>
<b>1</b>	30850023	Packaging	Including: export box, inner protection material
<b>2</b>	30850024	Export box	Excluding: inner protection material

### 10.2.5.2 Balances without draft shield

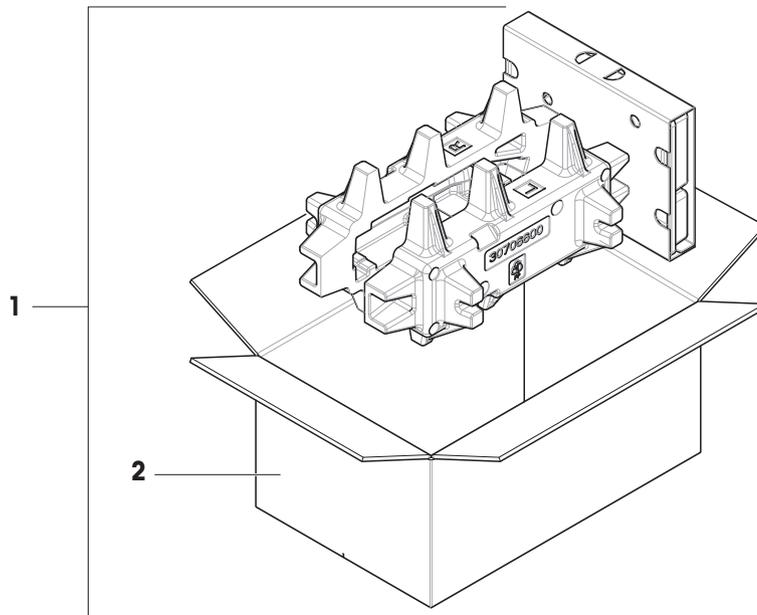

	<b>Order no.</b>	<b>Designation</b>	<b>Remarks</b>
<b>1</b>	30850037	Packaging	Including: export box, inner protection material
<b>2</b>	30850043	Export box	Excluding: inner protection material

## 11 Disposal

In conformance with the European Directive 2012/19/EU on Waste Electrical and Electronic Equipment (WEEE) this device may not be disposed of in domestic waste. This also applies to countries outside the EU, per their specific requirements.

Please dispose of this product in accordance with local regulations at the collecting point specified for electrical and electronic equipment. If you have any questions, please contact the responsible authority or the distributor from which you purchased this device. Should this device be passed on to other parties, the content of this regulation must also be related.



## 12 Compliance Information

National approval documents, e.g., the FCC Supplier Declaration of Conformity, are available online and/or included in the packaging.

▶ [www.mt.com/ComplianceSearch](http://www.mt.com/ComplianceSearch)

Contact METTLER TOLEDO for questions about the country-specific compliance of your instrument.

▶ [www.mt.com/contact](http://www.mt.com/contact)

### United States of America

This equipment has been tested and found to comply with the limits for a **Class A** digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions:

1. This device may not cause harmful interference.
2. This device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

# Index

## A

---

AC/DC adapter	111
acclimatization	
time	111
adjustment	46
external	47
setting	94
strategy	46
altitude	111
application	
back-weighing	44
check weighing	41
counting	40
density	45
dynamic weighing	42
formulation	43
totaling	44
weighing	36, 40
approved balance	64
automation	39

## B

---

back-weighing	44
balance	
reset	105
barcode reader	53
below-the-balance weighing	31
Bluetooth	50, 75
brightness	73

## C

---

certified balance	
see approved balance	64
check weighing	41
command	
MT-SICS	55, 59, 75
compliance information	132
configuration	
report	39
weighing	38
convention	7
counting	40

## D

---

density	45
---------	----

device	
barcode reader	53
edit setting	55
foot switch	53
keyboard	54
peripheral	50, 75
printer	51
dimension	116
disposal	131
door	
handle	15
draft shield	15
QuickLock	16
draft shield door	
QuickLock	16
draft shield panel	
release button	17
drip tray	15
drop to cursor	56, 59
dynamic weighing	42

## E

---

EasyDirect Balance	56, 60, 75
eccentricity test	
perform	49
setting	97
environmental condition	23, 111
Ethernet	50, 74
EULA	28
external	
adjustment	47
device	50, 75

## F

---

factory settings	105
foot switch	53
formulation	43

## H

---

history	66
humidity	111

## I

---

ID	37
install	
put into operation	27
site	23

interface	
Bluetooth	50, 75
Ethernet	50, 74

## K

keyboard	54
----------	----

## L

legal-for-trade balance	
see approved balance	64
level	
balance	28
indicator	18
leveling aid	66
leveling feet	16
leveling aid	66
leveling feet	16
LFT balance	
see approved balance	64
location	23
log in	63
log out	63

## M

MT-SICS	55, 59, 75
---------	------------

## O

overview	
terminal	14
type label	17

## P

pack	
balance	31
password	
reset	63
perform	
eccentricity test	49
repeatability test	48
sensitivity test	48
power consumption	
balance	111
power saving	14, 29
power supply	
see AC/CD adapter	111
print	
report	39
printer	51

profile	
weighing	35

## Q

QuickLock	
draft shield	16
draft shield door	16

## R

range	
tolerance	37
release button	
draft shield panel	17
repeatability test	
perform	48
setting	96
report	
configuration	39
print	39
reset	
balance	105
password	63
routine test	47

## S

safety information	10
sample ID	37
sensitivity test	
perform	48
setting	96
series	38
service	
drop to cursor	56, 59
EasyDirect Balance	56, 60, 75
MT-SICS	55, 59, 75
setting	
adjustment	94
eccentricity test	97
repeatability test	96
sensitivity test	96
test	95
software	
version	7
sound	
terminal	73
standby	14, 29
statistics	38

store	
balance	31
strategy	
adjustment	46
switch on/off	29
symbol	7
warning	10

## T

---

tare	14
target weight	37
temperature	111
acclimatization time	111
warm-up time	111
terminal	
brightness	73
overview	14
sound	73
test	47
setting	95
threshold	82
time	
acclimatization	111
warm up	111
tolerance	37
totaling	44
transport	
long distance	31
short distance	30
type label	
overview	17

## U

---

unpack	
balance	23
USB	
see device	50, 75

## W

---

warm up	
time	111
warning symbol	10
weighing	
application	36
configuration	38
profile	35
series	38
weighing pan	15

weight	
target	37

## Z

---

zero	14
------	----





## To protect your product's future:

METTLER TOLEDO Service assures the quality, measuring accuracy and preservation of value of this product for years to come.

Please request full details about our attractive terms of service.

► [www.mt.com/service](http://www.mt.com/service)

[www.mt.com/MR-balances](http://www.mt.com/MR-balances)

For more information

**Mettler-Toledo GmbH**

Im Langacher 44  
8606 Greifensee, Switzerland  
[www.mt.com/contact](http://www.mt.com/contact)

Subject to technical changes.  
© 12/2023 METTLER TOLEDO. All rights reserved.  
30491844A en



30491844